

Sample Name :N-Acetyl-Ser-Asp-Lys-Pro
 Cat. No. :RP10555
 Lot. No. :PE1761601

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

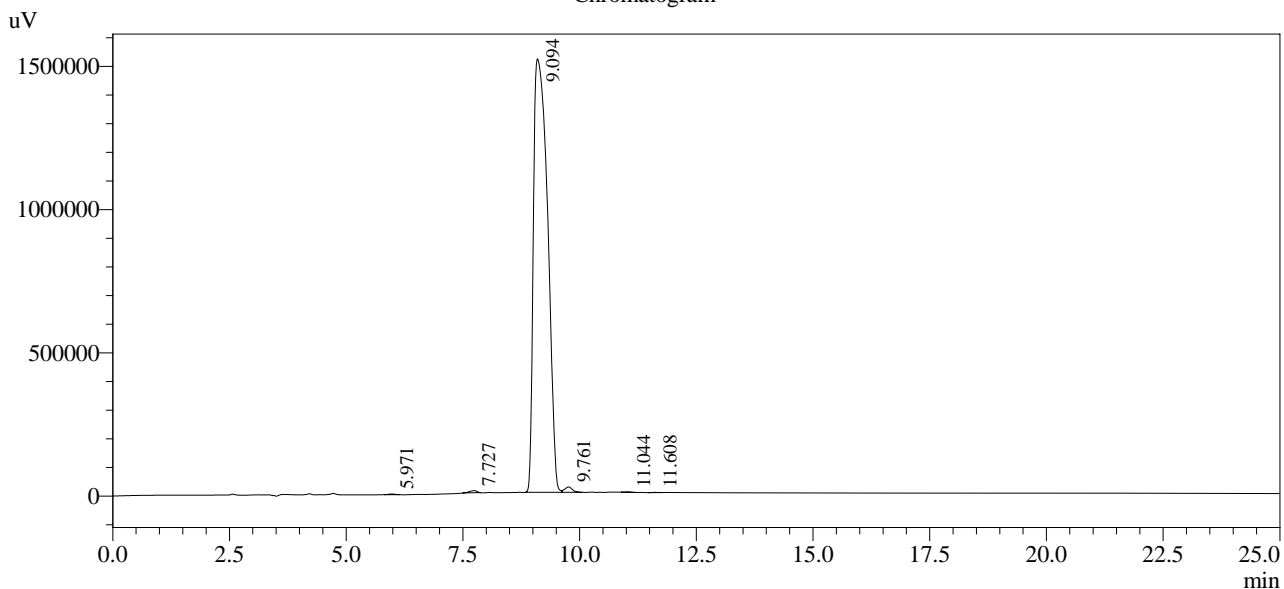

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.971	20101	2126	0.062
2	7.727	80969	7653	0.251
3	9.094	31871006	1513322	98.987
4	9.761	208763	18557	0.648
5	11.044	9697	1317	0.030
6	11.608	6501	975	0.020
Total		32197038	1543951	100.000