

Sample Name :Gly-Arg-Gly-Asp-Ser  
 Cat. No. : RP10848  
 Lot. No. : PE1071601

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

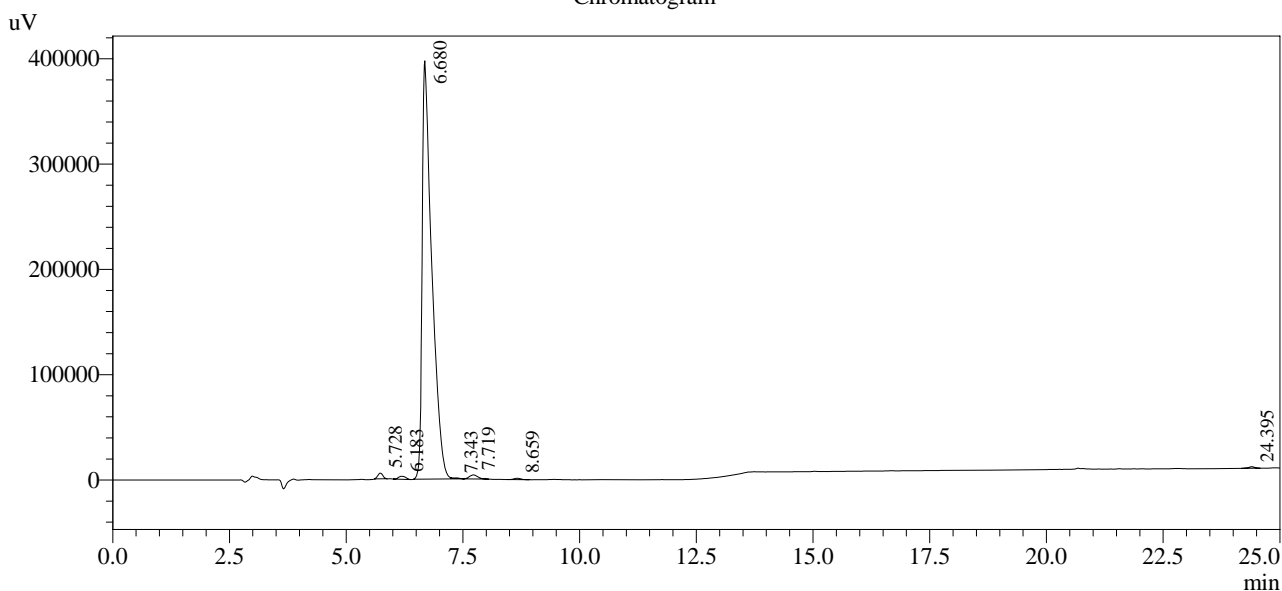

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.728	39977	5420	0.683
2	6.183	30695	2867	0.524
3	6.680	5699352	397311	97.346
4	7.343	10320	999	0.176
5	7.719	47578	3835	0.813
6	8.659	13857	1317	0.237
7	24.395	12936	1482	0.221
Total		5854715	413232	100.000