

Sample Name :Corticotropin Releasing Factor, human, rat
 Cat. No. :RP10982
 Lot. No. : PE8981603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

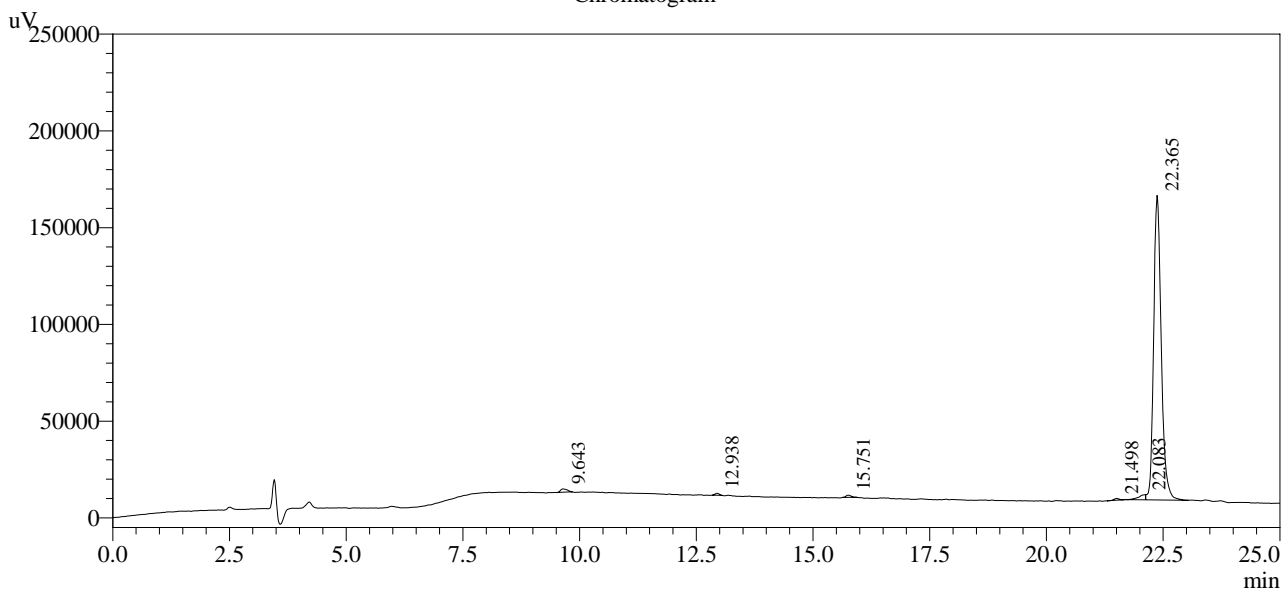

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.643	17117	1722	0.923
2	12.938	6336	1012	0.341
3	15.751	8602	1115	0.464
4	21.498	7009	936	0.378
5	22.083	28430	2589	1.532
6	22.365	1787877	157381	96.362
Total		1855372	164755	100.000