

Sample Name :Angiotensin II, human
 Cat. No. :RP11257
 Lot. No. : PE0091605

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

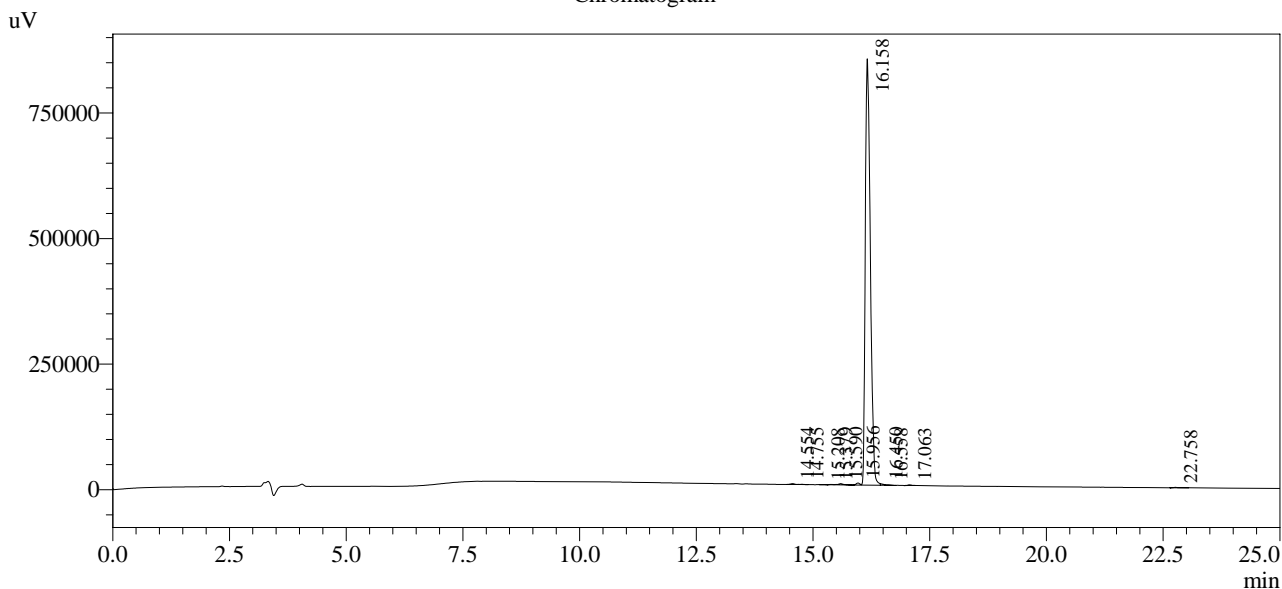

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.554	9116	1633	0.141
2	14.755	2190	441	0.034
3	15.208	2432	438	0.038
4	15.379	4325	857	0.067
5	15.590	20543	2428	0.317
6	15.956	21985	4078	0.339
7	16.158	6392808	848456	98.621
8	16.450	12087	2699	0.186
9	16.558	5210	717	0.080
10	17.063	6740	1333	0.104
11	22.758	4785	833	0.074
Total		6482220	863914	100.000