

Sample Name : Amyln.human.amide
 Cat. No. : RP11278
 Lot. No. : P8821603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
37.00	Pumps	Pump B Conc.	5	
37.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

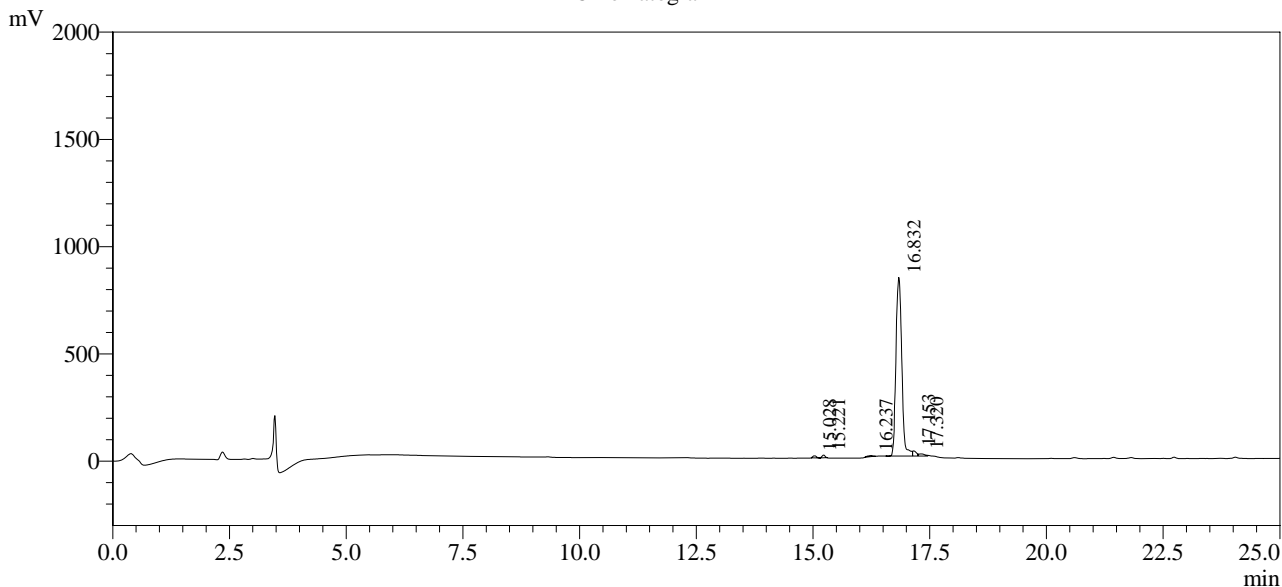

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.028	52317	10495	0.685
2	15.221	55301	12506	0.724
3	16.237	45134	5432	0.591
4	16.832	7268870	832475	95.119
5	17.153	125991	23762	1.649
6	17.320	94217	10032	1.233
Total		7641830	894702	100.000