

Sample Name : [Met<sup>5</sup>]-Enkephalin  
 Cat. No. : RP10886  
 Lot. No. : PE9011603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

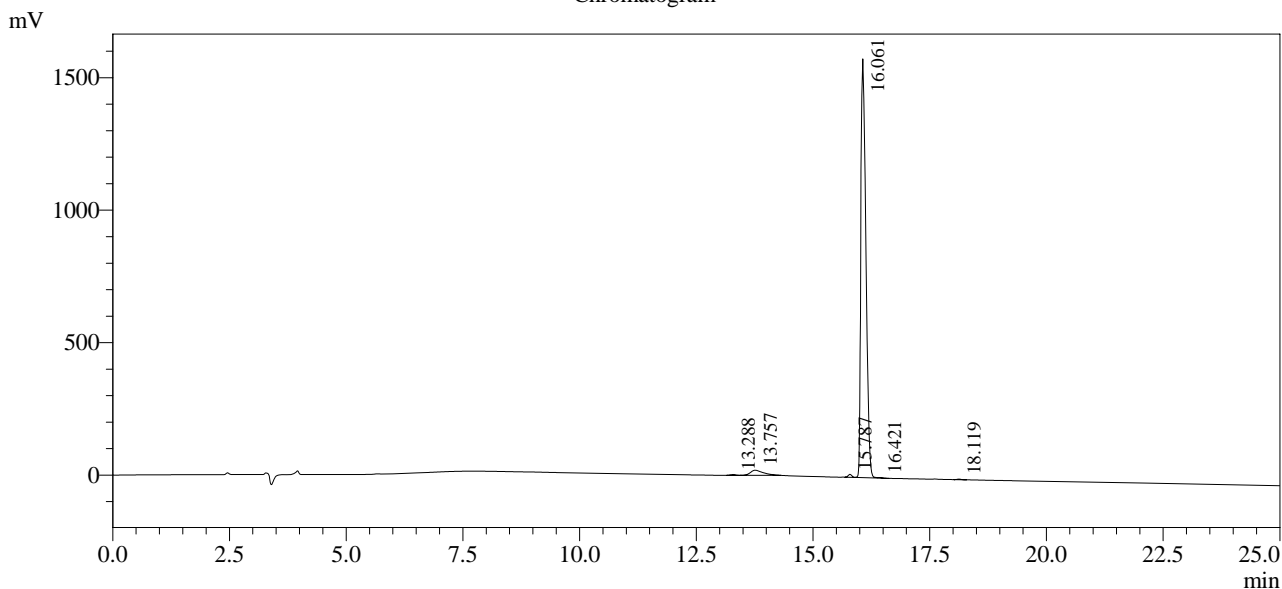

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.288	20723	2548	0.167
2	13.757	372850	19180	3.004
3	15.787	58437	11021	0.471
4	16.061	11937447	1580571	96.165
5	16.421	11600	1891	0.093
6	18.119	12484	2255	0.101
Total		12413540	1617467	100.000