

Sample Name : SIYRY  
Cat. No. : RP20234  
Lot. No. : PE8011604

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

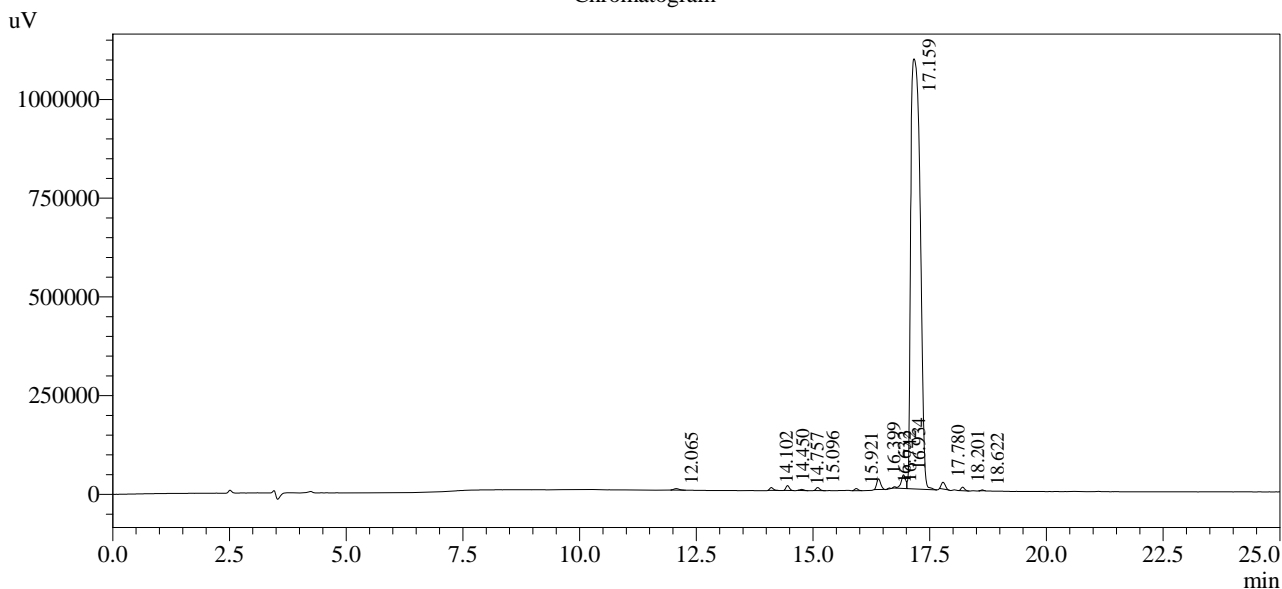

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.065	31735	3834	0.198
2	14.102	37409	7198	0.233
3	14.450	62910	12138	0.392
4	14.757	15652	2778	0.097
5	15.096	42729	7833	0.266
6	15.921	27403	5297	0.171
7	16.399	161588	27212	1.006
8	16.632	7522	2032	0.047
9	16.742	12873	3430	0.080
10	16.934	229858	34647	1.432
11	17.159	15266562	1088947	95.090
12	17.780	102265	17321	0.637
13	18.201	47886	8956	0.298
14	18.622	8433	2053	0.053
Total		16054827	1223675	100.000