

Sample Name :Proctolin
 Cat. No. :RP10475
 Lot. No. : PE6281608

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

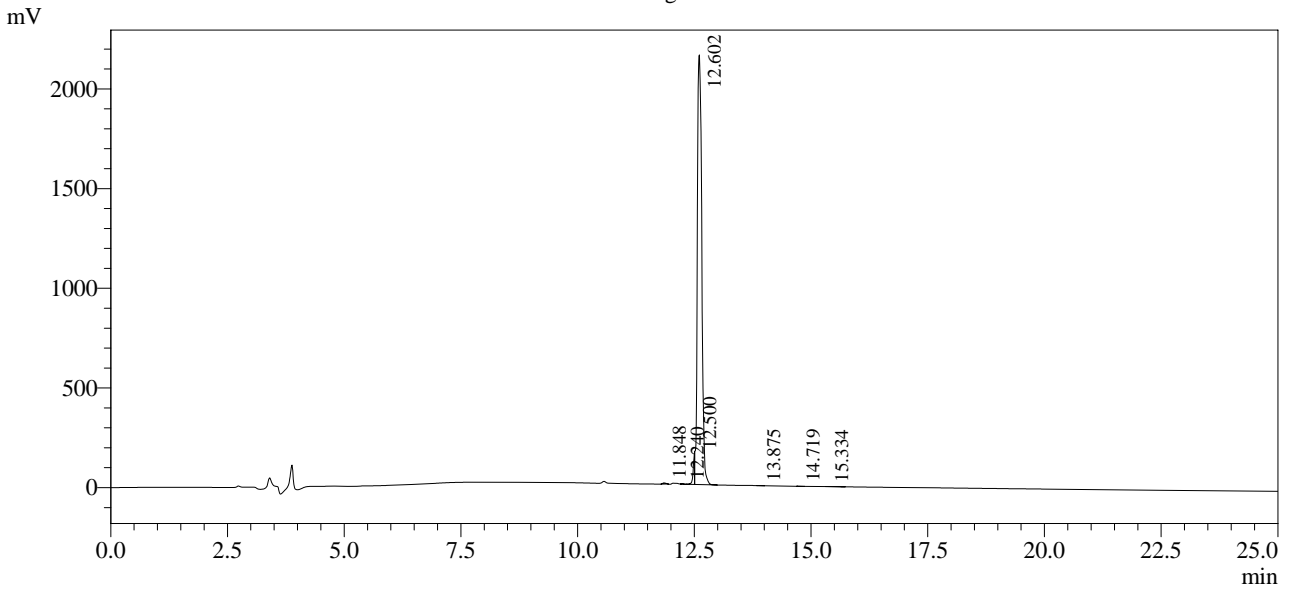

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.848	27111	5602	0.185
2	12.240	5494	1545	0.038
3	12.500	374747	153542	2.561
4	12.602	14221019	2155696	97.175
5	13.875	2473	568	0.017
6	14.719	1030	184	0.007
7	15.334	2548	79	0.017
Total		14634421	2317216	100.000