

Sample Name : Arg-Gly-Asp-Cys
 Cat. No. : RP10860
 Lot. No. : PE0211604


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

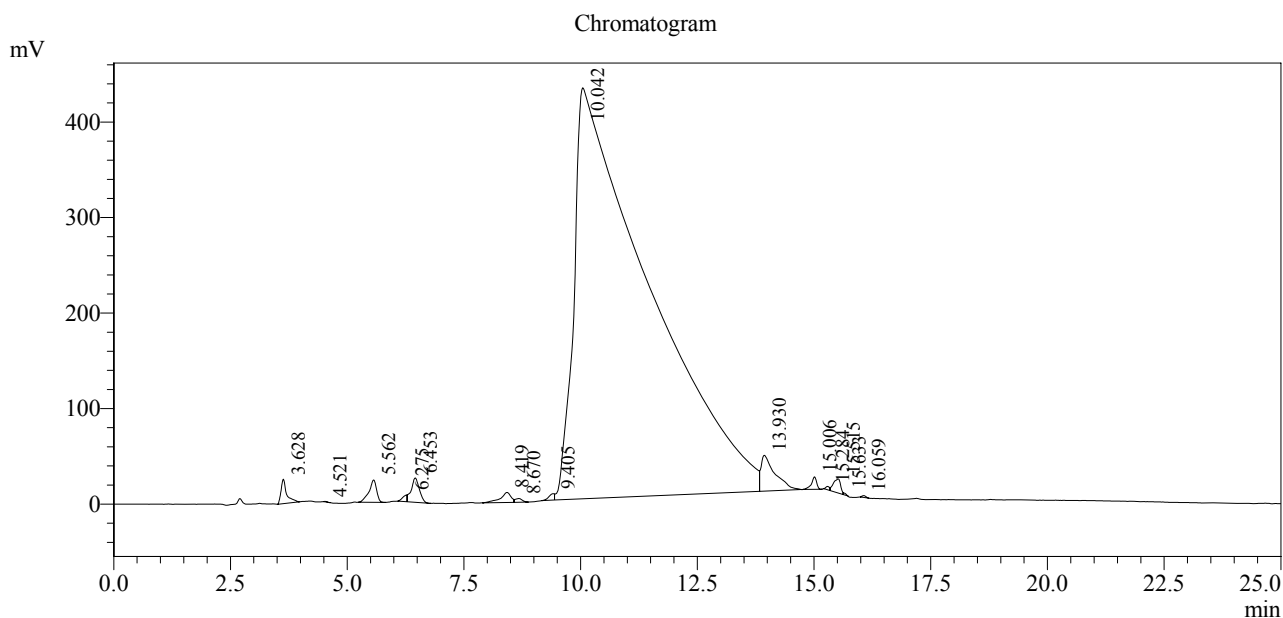

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	3.628	215292	25654	0.430
2	4.521	1920	415	0.004
3	5.562	266960	23500	0.533
4	6.275	46106	7086	0.092
5	6.453	307537	25512	0.615
6	8.419	164010	10522	0.328
7	8.670	40027	3923	0.080
8	9.405	54941	6646	0.110
9	10.042	47878616	430300	95.674
10	13.930	779108	37501	1.557
11	15.006	100658	13078	0.201
12	15.284	19704	3456	0.039
13	15.515	152142	14726	0.304
14	15.633	6414	1783	0.013
15	16.059	10161	1781	0.020
Total		50043596	605883	100.000