

Sample Name : Gastrin,human  
 Cat. No. : RP12740  
 Lot. No. : PE7601606

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
40.00	Pumps	Pump B Conc.	15	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

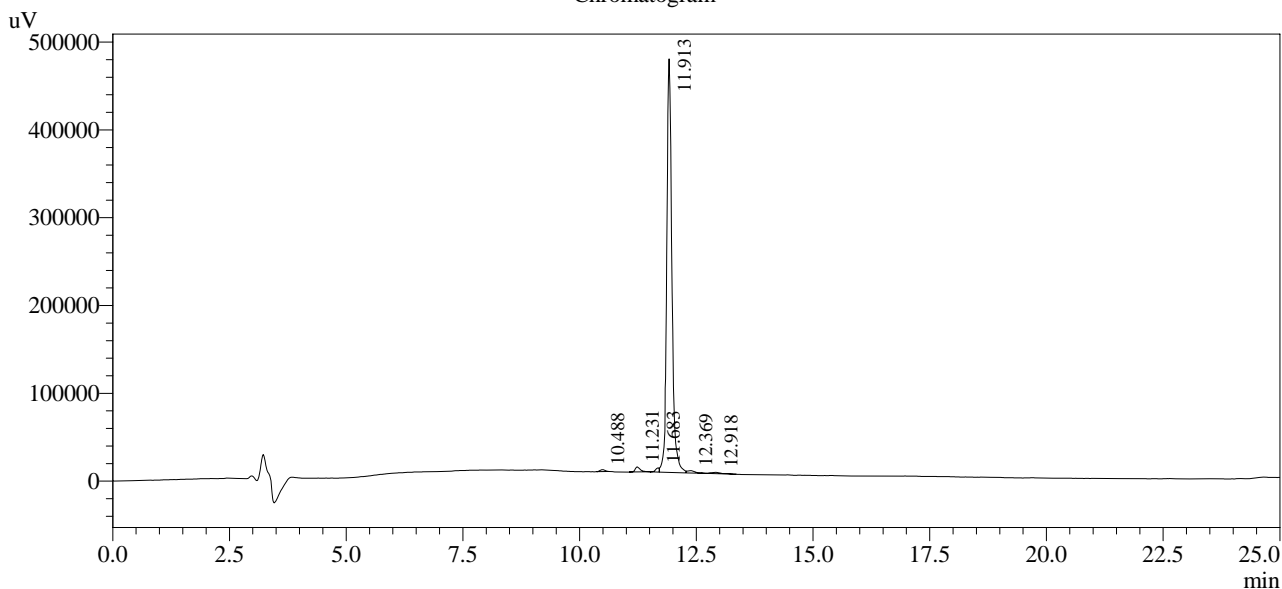

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.488	15567	2112	0.414
2	11.231	44275	5796	1.177
3	11.683	26018	4707	0.692
4	11.913	3617918	470988	96.194
5	12.369	30258	2727	0.805
6	12.918	27026	1579	0.719
Total		3761063	487909	100.000