

Sample Name : [Met<sup>5</sup>]-Enkephalin  
 Cat. No. : RP10886  
 Lot. No. : PE1711608

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

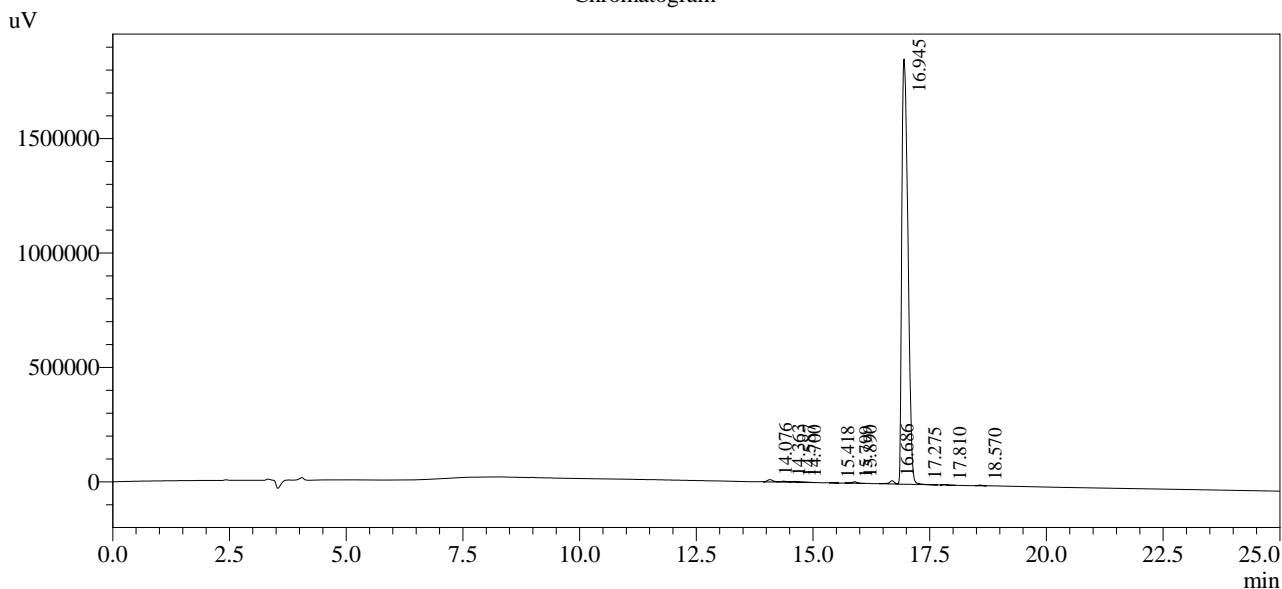

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.076	88652	9990	0.508
2	14.363	43779	4198	0.251
3	14.587	32959	3490	0.189
4	14.700	26349	2216	0.151
5	15.418	3540	674	0.020
6	15.799	14568	3266	0.083
7	15.890	41710	6938	0.239
8	16.686	105431	14332	0.604
9	16.945	17054009	1859238	97.641
10	17.275	22532	3805	0.129
11	17.810	15426	2897	0.088
12	18.570	17137	2959	0.098
Total		17466092	1914004	100.000