

Sample Name : Galanin,human  
 Cat. No. : RP10801  
 Lot. No. : PE9001603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<检测器 A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

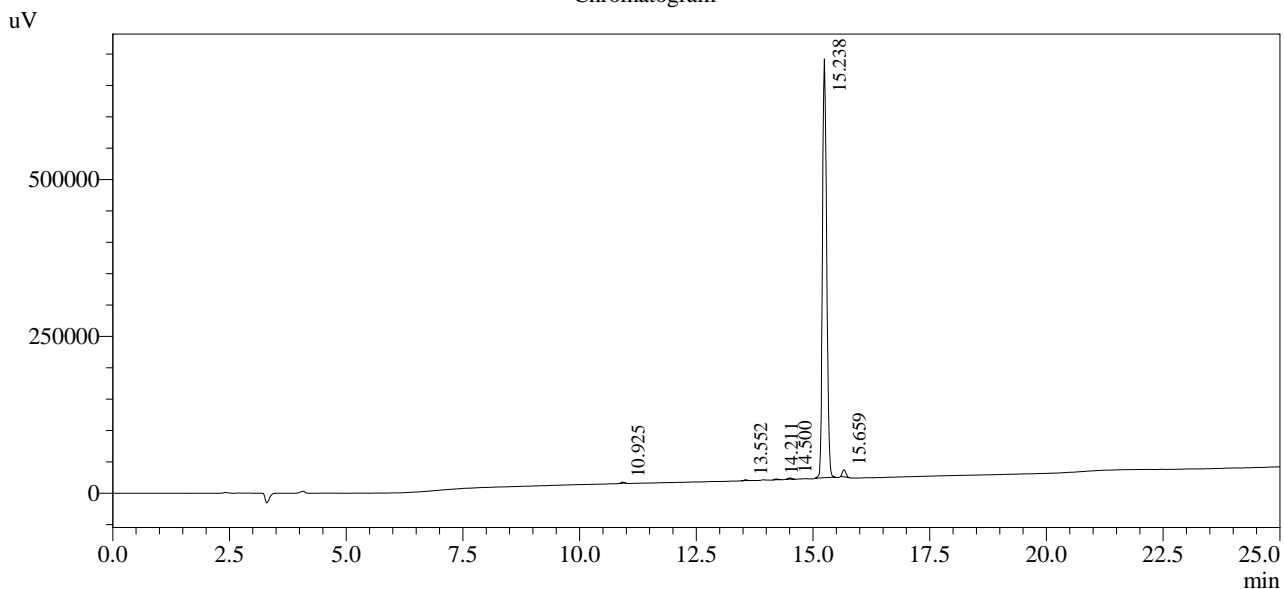

I Det.A Ch1 / 220nm

Peak Table

检测器 A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.925	6044	1452	0.141
2	13.552	6315	1367	0.147
3	14.211	5703	1259	0.133
4	14.500	9528	1920	0.222
5	15.238	4210922	667662	98.003
6	15.659	58200	11259	1.355
Total		4296712	684919	100.000