

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE0221601

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

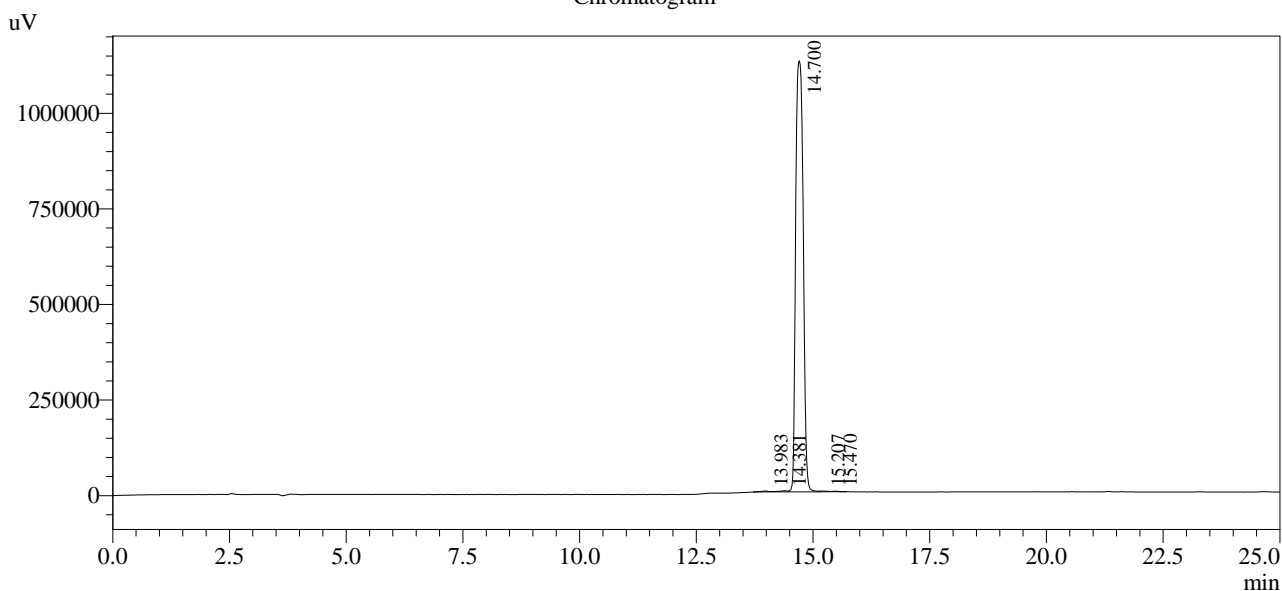

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.983	27513	2233	0.215
2	14.381	40541	2965	0.317
3	14.700	12690181	1127391	99.183
4	15.207	25613	1934	0.200
5	15.470	10816	1470	0.085
Total		12794664	1135993	100.000