

Sample Name : Lactoferrin (17-41)  
 Cat. No. : RP20489  
 Lot. No. : PE0281609

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

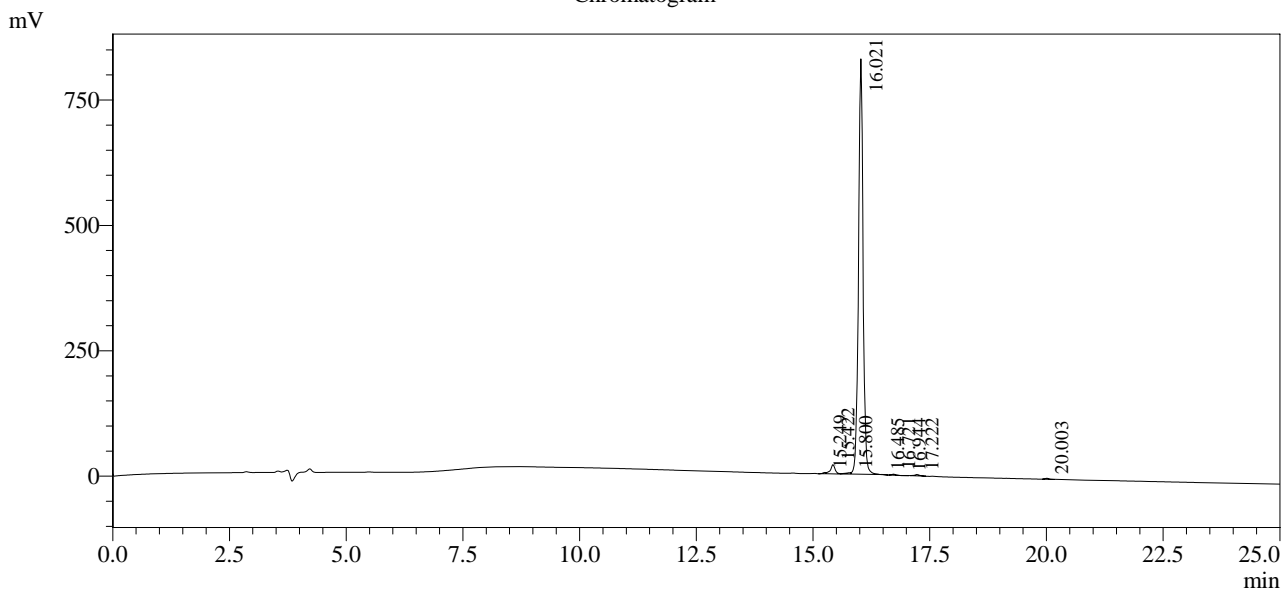

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.249	12030	2501	0.205
2	15.422	126237	18609	2.154
3	15.800	21953	2575	0.375
4	16.021	5654610	828273	96.464
5	16.485	1586	353	0.027
6	16.721	13620	2276	0.232
7	16.944	1185	269	0.020
8	17.222	19375	2703	0.331
9	20.003	11273	1935	0.192
Total		5861869	859495	100.000