

Sample Name : $\beta$ -amyloid (1-16)  
 Cat. No. : RP20103  
 Lot. No. : PE4091904  
 Time Processed : 9:23:27  
 Month-Day-Year Processed : 04/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
32.00	Pumps	Pump B Conc.	95	
32.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
41.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

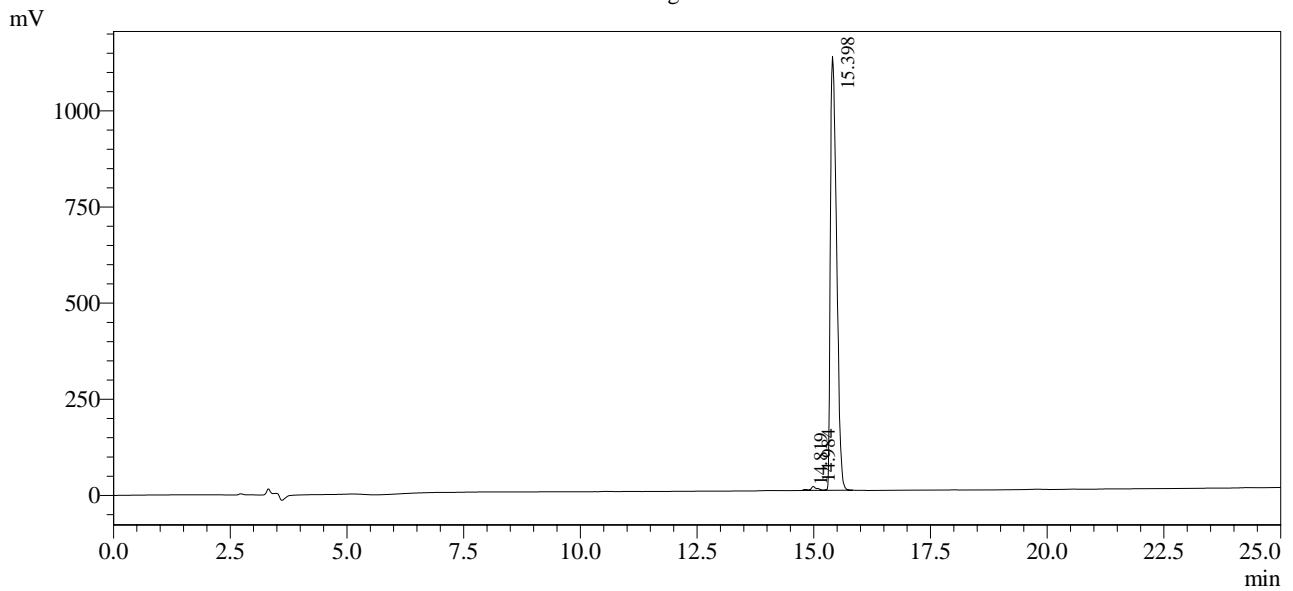

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.819	10851	1951	0.103
2	14.984	78425	9768	0.743
3	15.398	10463215	1128694	99.154
Total		10552490	1140413	100.000