

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : PE2301706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

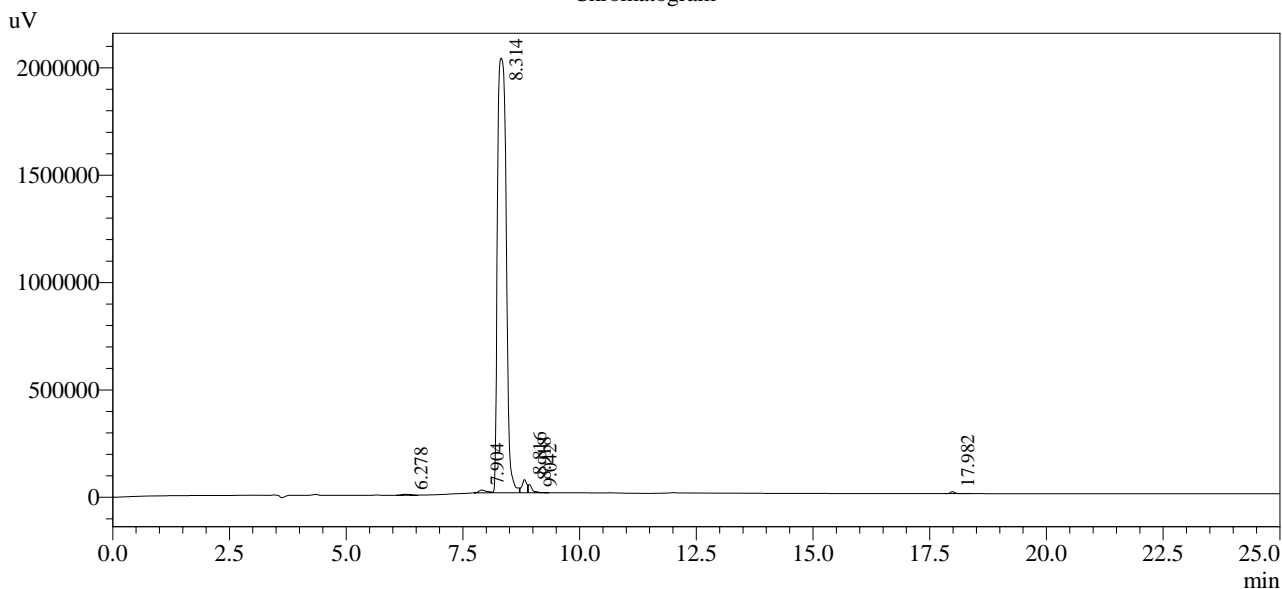

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.278	45342	4282	0.166
2	7.904	154939	13382	0.567
3	8.314	26363324	2024895	96.557
4	8.816	445629	61385	1.632
5	8.918	201377	38397	0.738
6	9.042	32524	5430	0.119
7	17.982	60257	9336	0.221
Total		27303394	2157108	100.000