

Sample Name :Angiotensin II, human
 Cat No. :RP11257
 Lot No. :E2126519L
 Time Processed :3:17:36 AM
 Month-Day-Year Processed :12/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

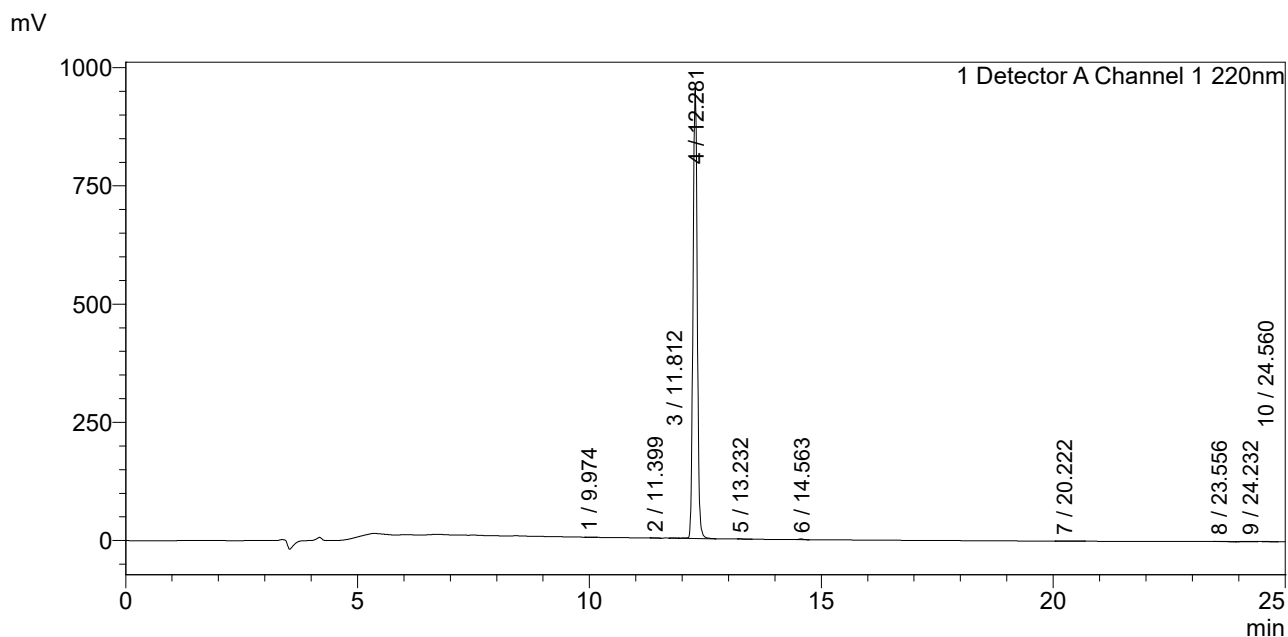

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.974	1326	227	0.022
2	11.399	2654	437	0.044
3	11.812	2096	341	0.035
4	12.281	6035375	952497	99.569
5	13.232	1319	104	0.022
6	14.563	9900	1629	0.163
7	20.222	2287	211	0.038
8	23.556	2013	143	0.033
9	24.232	3240	165	0.053
10	24.560	1271	141	0.021
Total		6061480	955895	100.000