

Sample Name :Protease-Activated Receptor-2, amide  
 Cat. No. :RP20334  
 Lot. No. :PE3061901  
 Time Processed :10:28:20  
 Month-Day-Year Processed :02/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

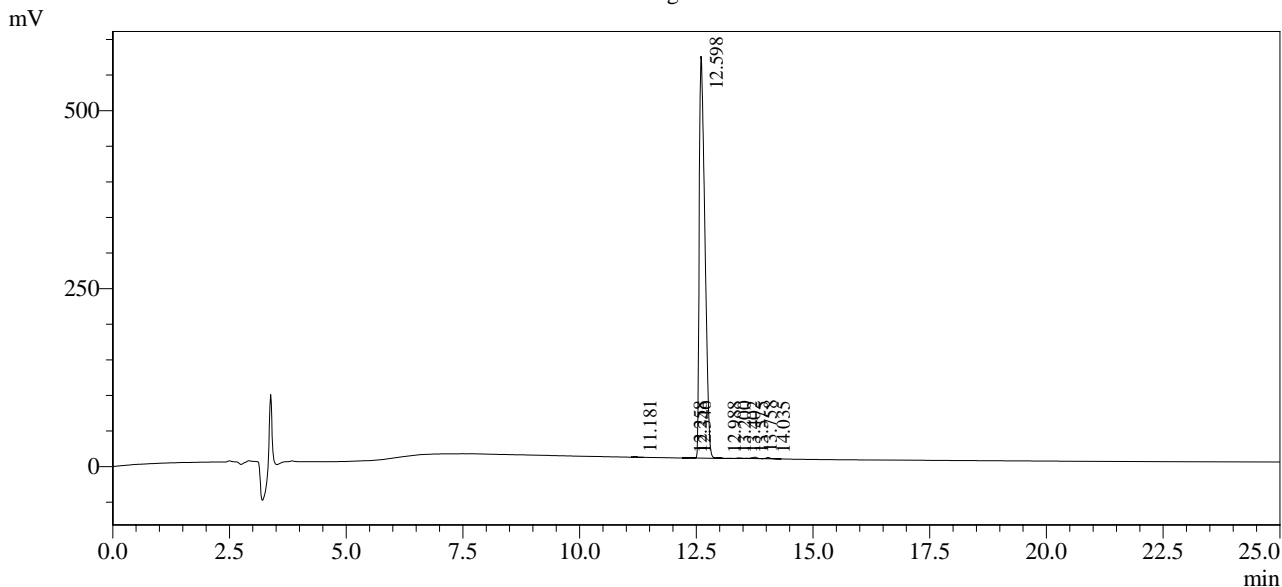

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.181	6160	1094	0.128
2	12.258	1142	281	0.024
3	12.346	1402	312	0.029
4	12.598	4762176	564542	99.050
5	12.988	2979	690	0.062
6	13.200	1894	373	0.039
7	13.402	5240	693	0.109
8	13.575	1900	392	0.040
9	13.758	13626	1904	0.283
10	14.035	11309	1783	0.235
Total		4807829	572064	100.000