

Sample Name :N-Acetyl- α -Endorphin
 Cat No.: RP11333
 Lot No.: E4725619I
 Time Processed:10:46:17
 Month-Day-Year Processed:09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

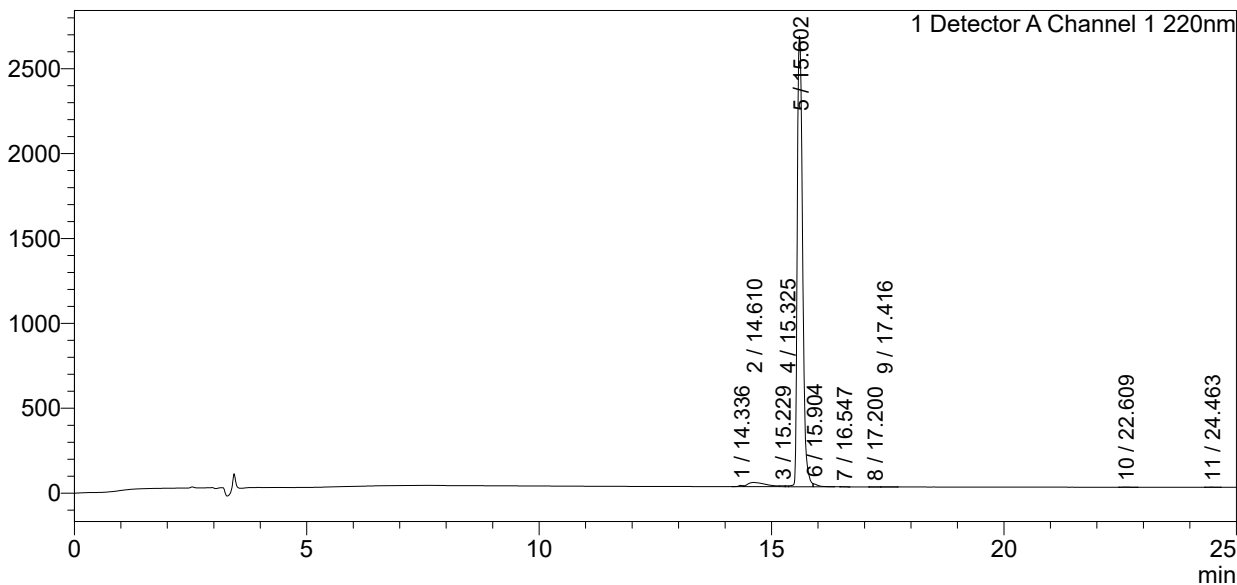

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.336	47802	7515	0.217
2	14.610	667698	25062	3.029
3	15.229	38286	5501	0.174
4	15.325	21342	4832	0.097
5	15.602	21129452	2654246	95.838
6	15.904	118358	17750	0.537
7	16.547	3879	743	0.018
8	17.200	3073	323	0.014
9	17.416	4355	541	0.020
10	22.609	8001	1071	0.036
11	24.463	4695	617	0.021
Total		22046942	2718200	100.000