

Sample Name :Kallikrein Inhibitor
 Cat. No. : RP10161
 Lot. No. : E4689719I
 Time Processed :13:45:05
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

Chromatogram

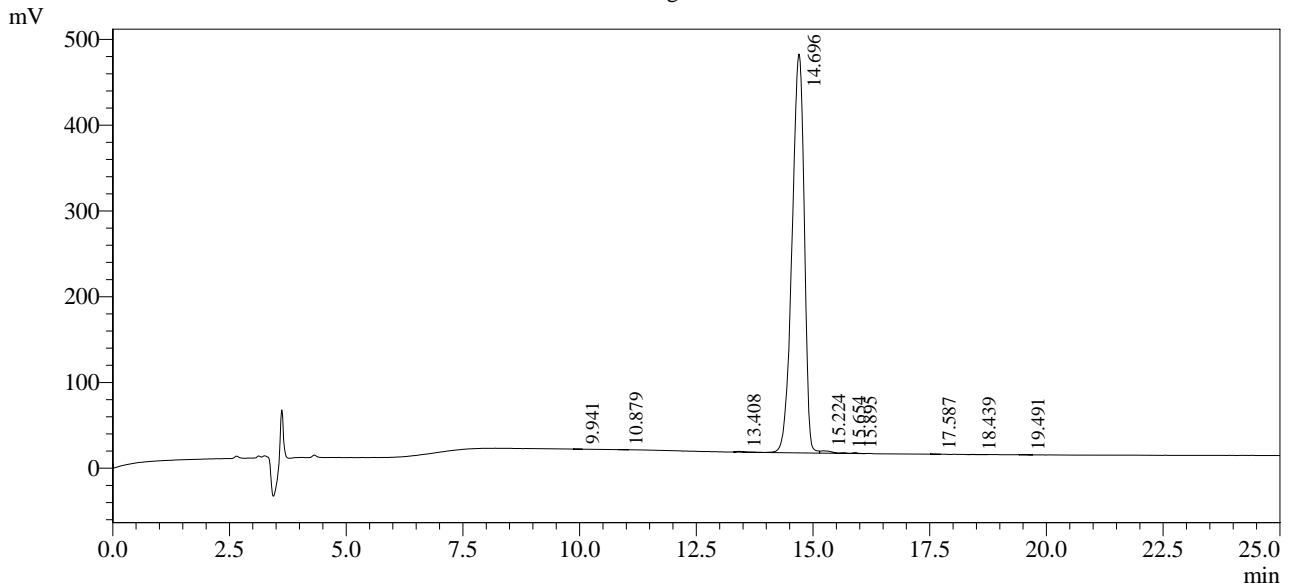

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.941	1034	205	0.012
2	10.879	1002	168	0.012
3	13.408	9922	970	0.117
4	14.696	8405973	465171	99.146
5	15.224	42728	2586	0.504
6	15.654	5704	653	0.067
7	15.895	8077	1061	0.095
8	17.587	1126	169	0.013
9	18.439	1531	131	0.018
10	19.491	1302	159	0.015
Total		8478399	471273	100.000