

Sample Name :Kemptide
 Cat No. : RP10287
 Lot No. : E3671820G
 Time Processed : 6:46:06
 Month-Day-Year Processed : 07/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

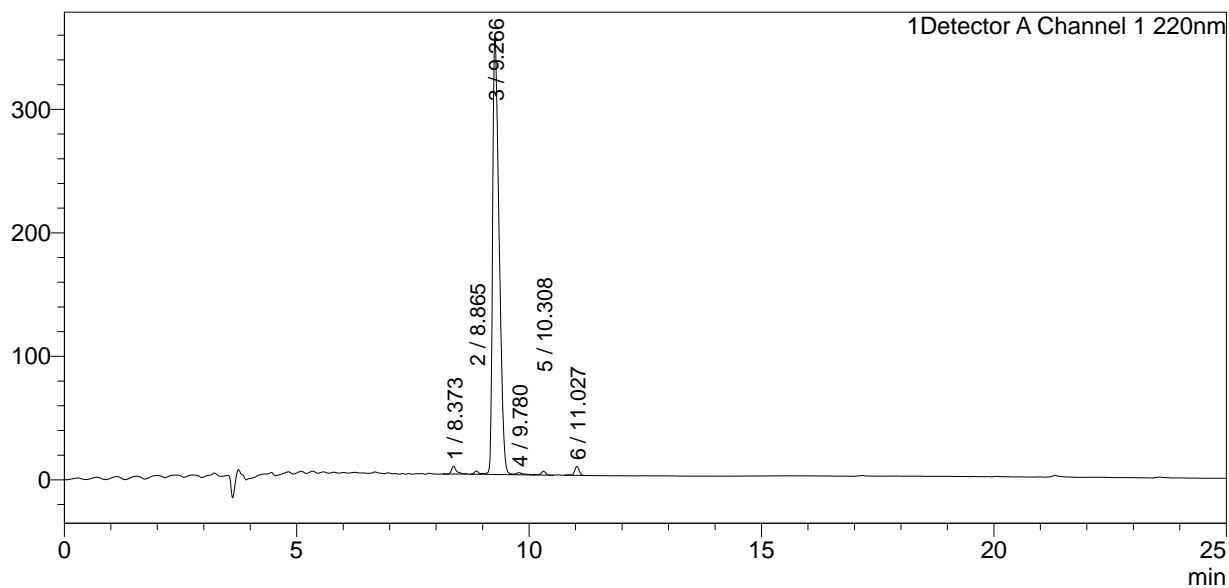

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.373	45296	6209	1.264
2	8.865	16525	2673	0.461
3	9.266	3435006	352440	95.846
4	9.780	15972	1665	0.446
5	10.308	21244	2995	0.593
6	11.027	49844	7242	1.391
Total		3583887	373225	100.000