

Sample Name :Substance P, Free Acid
 Cat No. :RP10185
 Lot No. :E2914219G
 Time Processed :3:51:24
 Month-Day-Year Processed :07/22/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

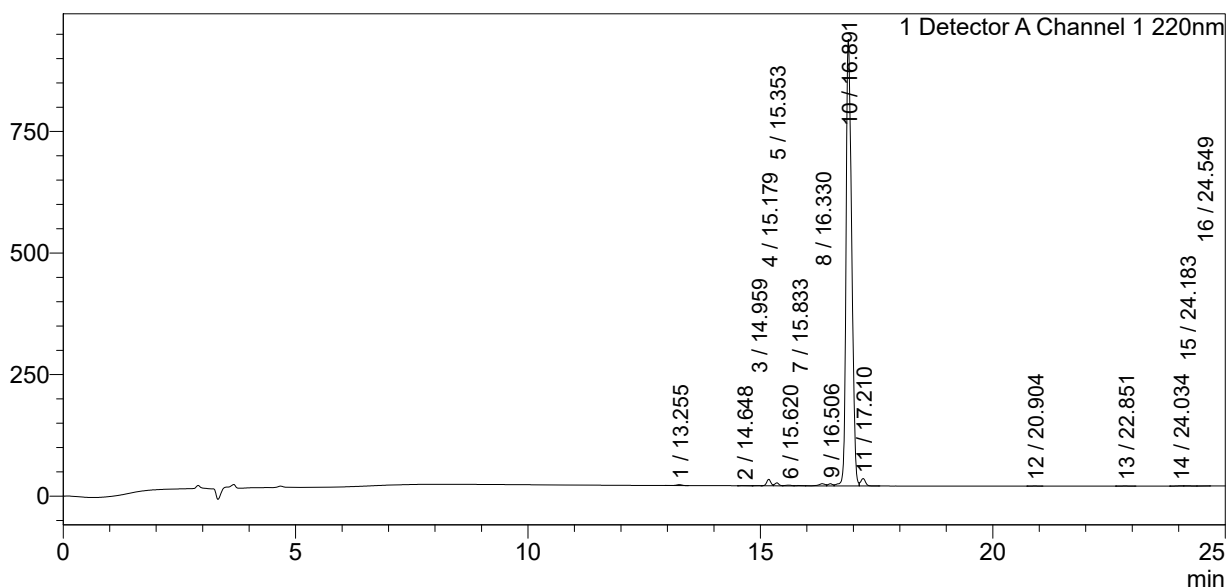

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.255	15980	1841	0.198
2	14.648	2751	432	0.034
3	14.959	2808	432	0.035
4	15.179	84159	13450	1.043
5	15.353	38490	6285	0.477
6	15.620	14033	1458	0.174
7	15.833	8621	888	0.107
8	16.330	46959	4555	0.582
9	16.506	31030	4504	0.385
10	16.891	7692391	918379	95.347
11	17.210	108884	15369	1.350
12	20.904	3618	372	0.045
13	22.851	3667	335	0.045
14	24.034	5628	609	0.070
15	24.183	6669	660	0.083

Peak#	Ret. Time	Area	Height	Area%
16	24.549	2104	196	0.026
Total		8067793	969766	100.000