

Sample Name : β -Amyloid (1-9)
 Cat No. : RP20160
 Lot No. : E4724220K
 Time Processed : 8:01:57 AM
 Month-Day-Year Processed : 11/17/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010140

<Chromatogram>

mV

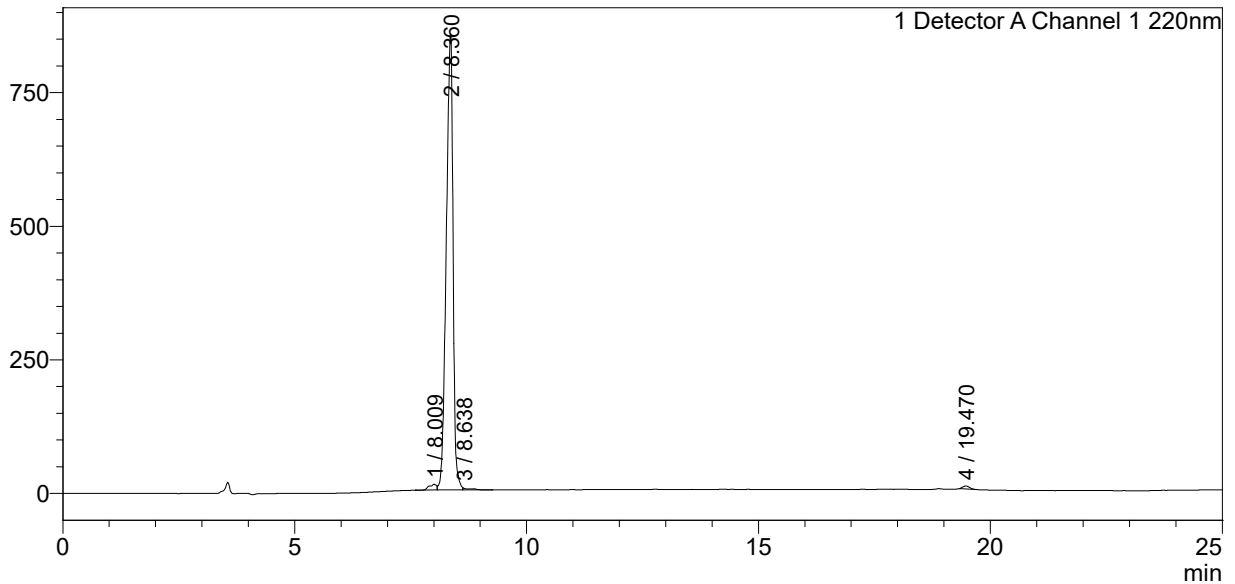

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.009	116970	10832	1.323
2	8.360	8634273	853901	97.628
3	8.638	37182	3627	0.420
4	19.470	55669	5572	0.629
Total		8844094	873931	100.000