

Sample Name :Bradykinin (1-7)
 Cat No: RP11133
 Lot No : E4397221H
 Time Processed :23:12:07
 Month-Day-Year Processed :08/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

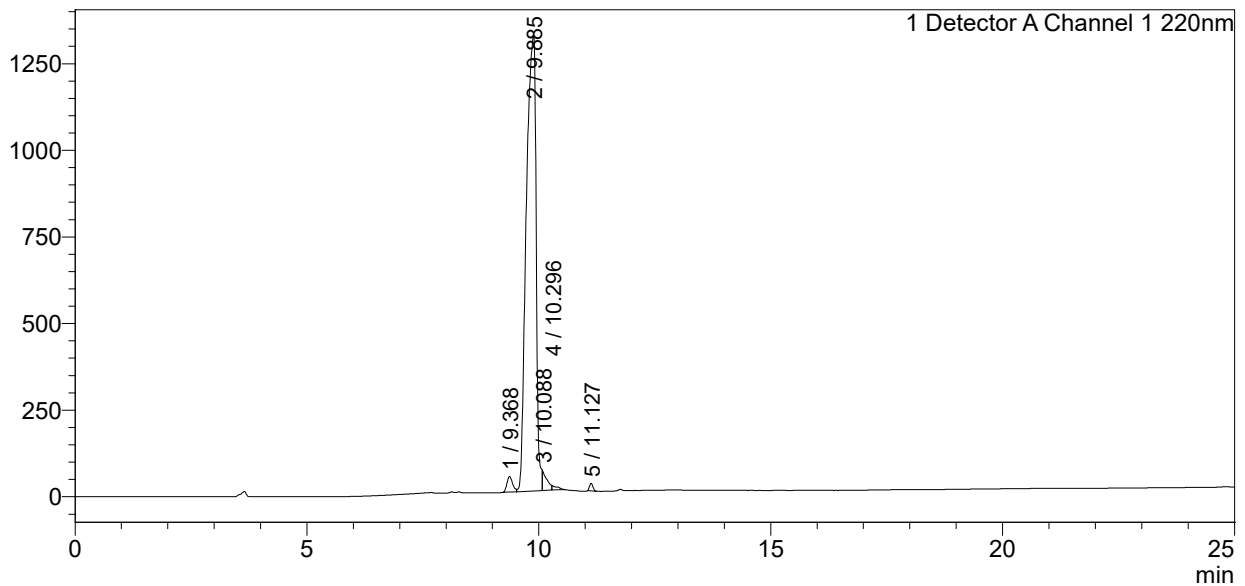

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 9.368 | 384396 | 45113 | 1.904 |
| 2 | 9.885 | 19213542 | 1314333 | 95.186 |
| 3 | 10.088 | 381451 | 56355 | 1.890 |
| 4 | 10.296 | 96481 | 12286 | 0.478 |
| 5 | 11.127 | 109475 | 21700 | 0.542 |
| Total | | 20185345 | 1449787 | 100.000 |