


Mass Spectrum

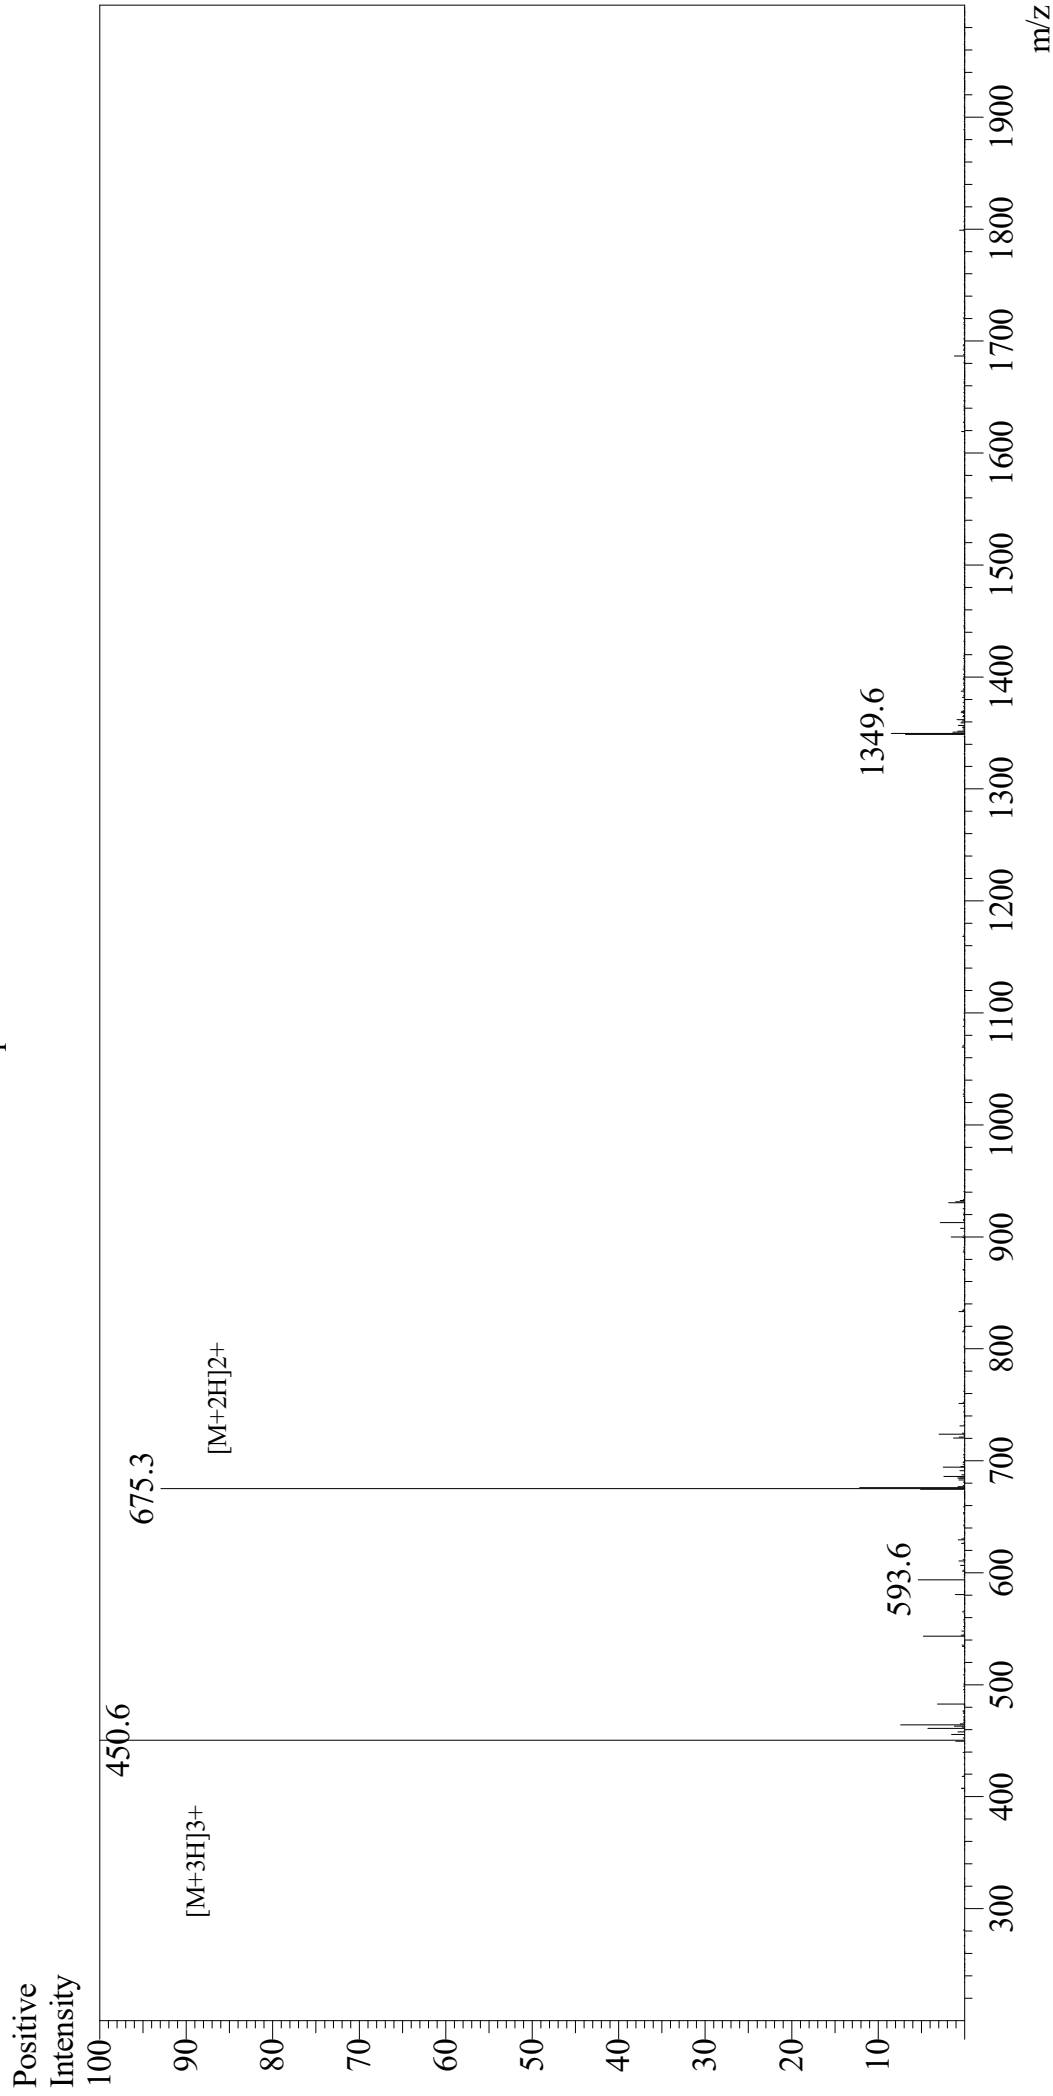

Sample Information

User : Gary
Month-Day Processed : 02/20/19
Time Processed : 10:44:20 AM
Injection Volume : 0.2
Sample Name : BDC2.5 mimotope 1040-31
Cat No. : RP20518
Lot No. : PE3451902
Theoretical MW : 1348.60
Observed MW : 1348.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH