

Sample Name :Transportan  
 Cat No: RP20512  
 Lot No : E4726220K  
 Time Processed :11:41:18 AM  
 Month-Day-Year Processed :11/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

### <Chromatogram>

mV

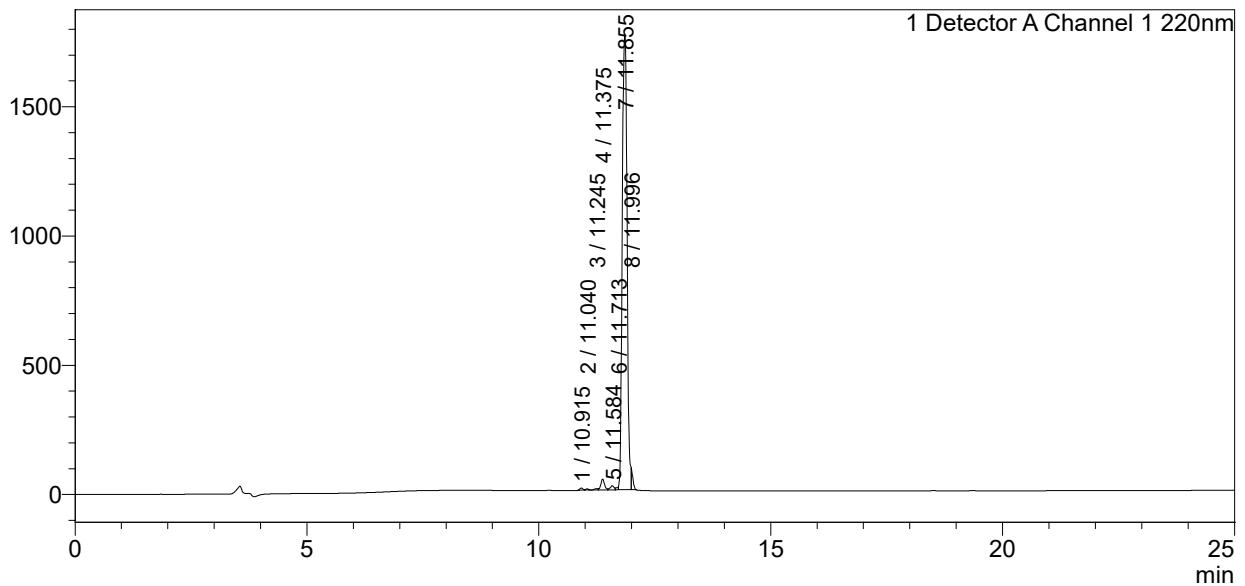

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.915	31552	7976	0.237
2	11.040	20130	4863	0.151
3	11.245	28079	4879	0.211
4	11.375	231712	42444	1.743
5	11.584	90873	15888	0.684
6	11.713	34564	10065	0.260
7	11.855	12674689	1757193	95.345
8	11.996	181964	84209	1.369
Total		13293563	1927516	100.000