

Sample Name :Systemin  
 Cat No.: RP10622  
 Lot No.: PE5091905  
 Time Processed :14:04:01  
 Month-Day-Year Processed :05/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
25.00	Pumps	Solvent B Conc.	60
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010509

### <Chromatogram>

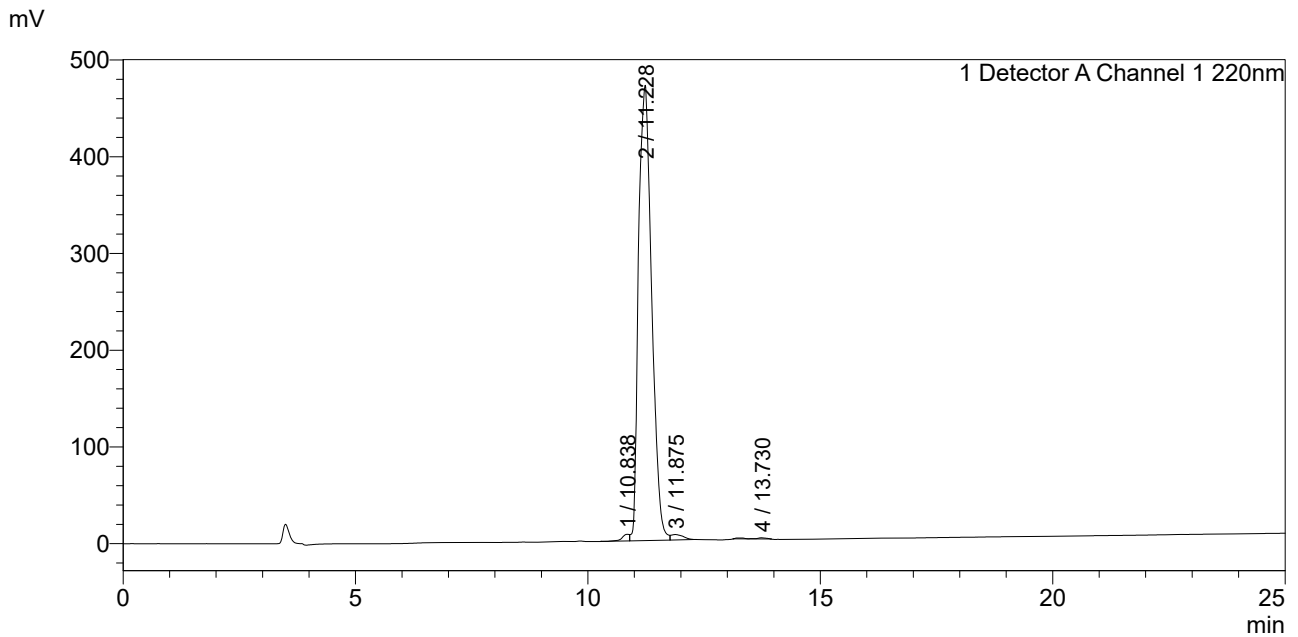

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.838	74827	6867	0.794
2	11.228	9211683	470605	97.808
3	11.875	100856	5594	1.071
4	13.730	30732	1249	0.326
Total		9418098	484315	100.000