

Sample Name :Glucagon-Like Peptide (GLP) II, human
 Cat No.: RP10769
 Lot No.:E4757219I
 Time Processed :12:51:43
 Month-Day-Year Processed :10/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
10.00	Pumps	Solvent B Conc.	35
35.00	Pumps	Solvent B Conc.	95
37.00	Pumps	Solvent B Conc.	95
37.01	Pumps	Solvent B Conc.	5
43.00	Pumps	Solvent B Conc.	5
43.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

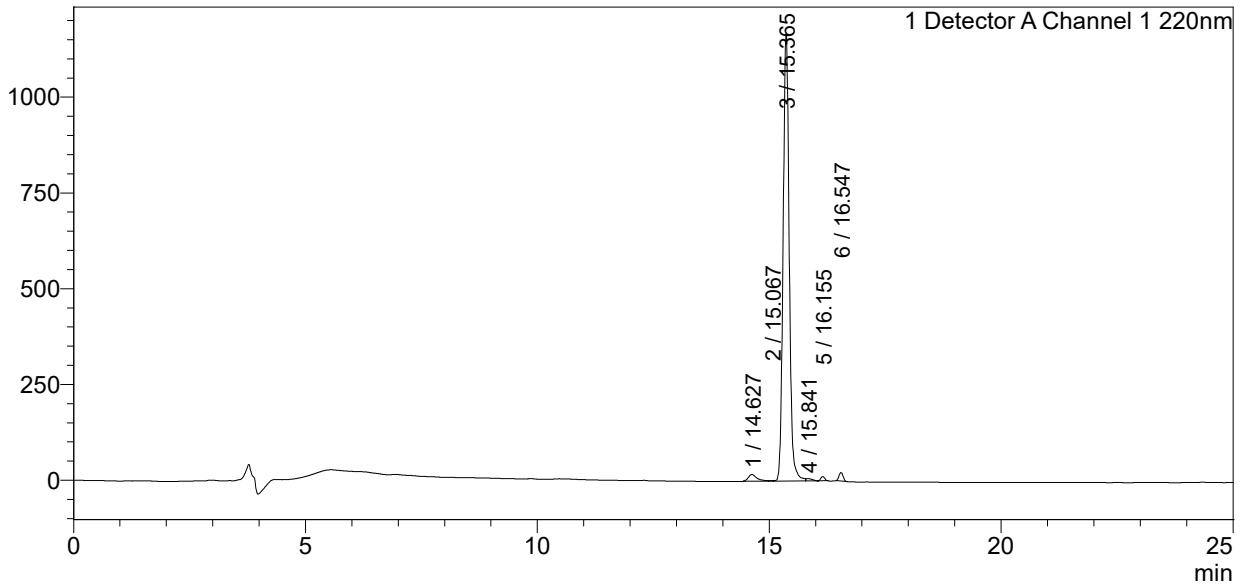

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.627	227177	17547	2.017
2	15.067	7131	1257	0.063
3	15.365	10721172	1169861	95.172
4	15.841	53395	5966	0.474
5	16.155	63351	10853	0.562
6	16.547	136773	22461	1.214
7	34.463	56067	6394	0.498
Total		11265066	1234339	100.000