

Sample Name : Bradykinin  
 Cat. No. : RP11129  
 Lot. No. : PE3451902  
 Time Processed :17:30:40  
 Month-Day-Year Processed :02/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

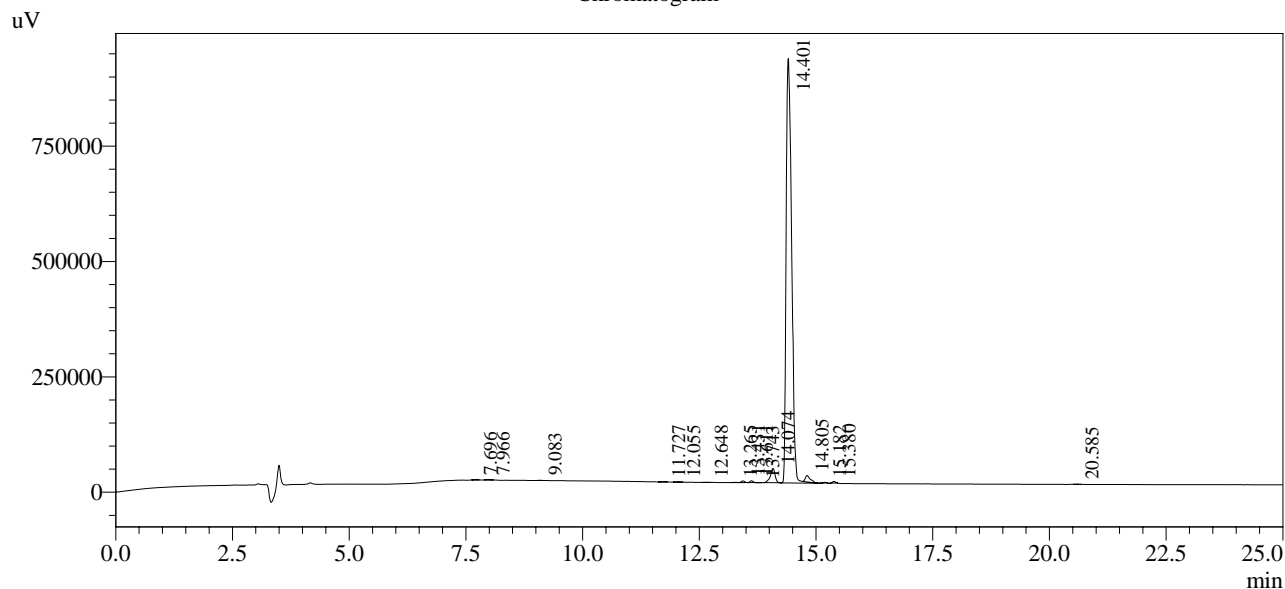

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.696	2081	466	0.026
2	7.966	3667	594	0.046
3	9.083	2459	464	0.031
4	11.727	1746	348	0.022
5	12.055	1571	275	0.020
6	12.648	1261	203	0.016
7	13.265	2513	503	0.032
8	13.431	18007	3647	0.227
9	13.611	17685	3872	0.223
10	13.743	638	195	0.008
11	14.074	212966	30858	2.690
12	14.401	7524751	920335	95.043
13	14.805	102067	13956	1.289
14	15.182	7475	1654	0.094
15	15.380	16203	3469	0.205
16	20.585	2127	458	0.027
Total		7917217	981297	100.000