


Mass Spectrum

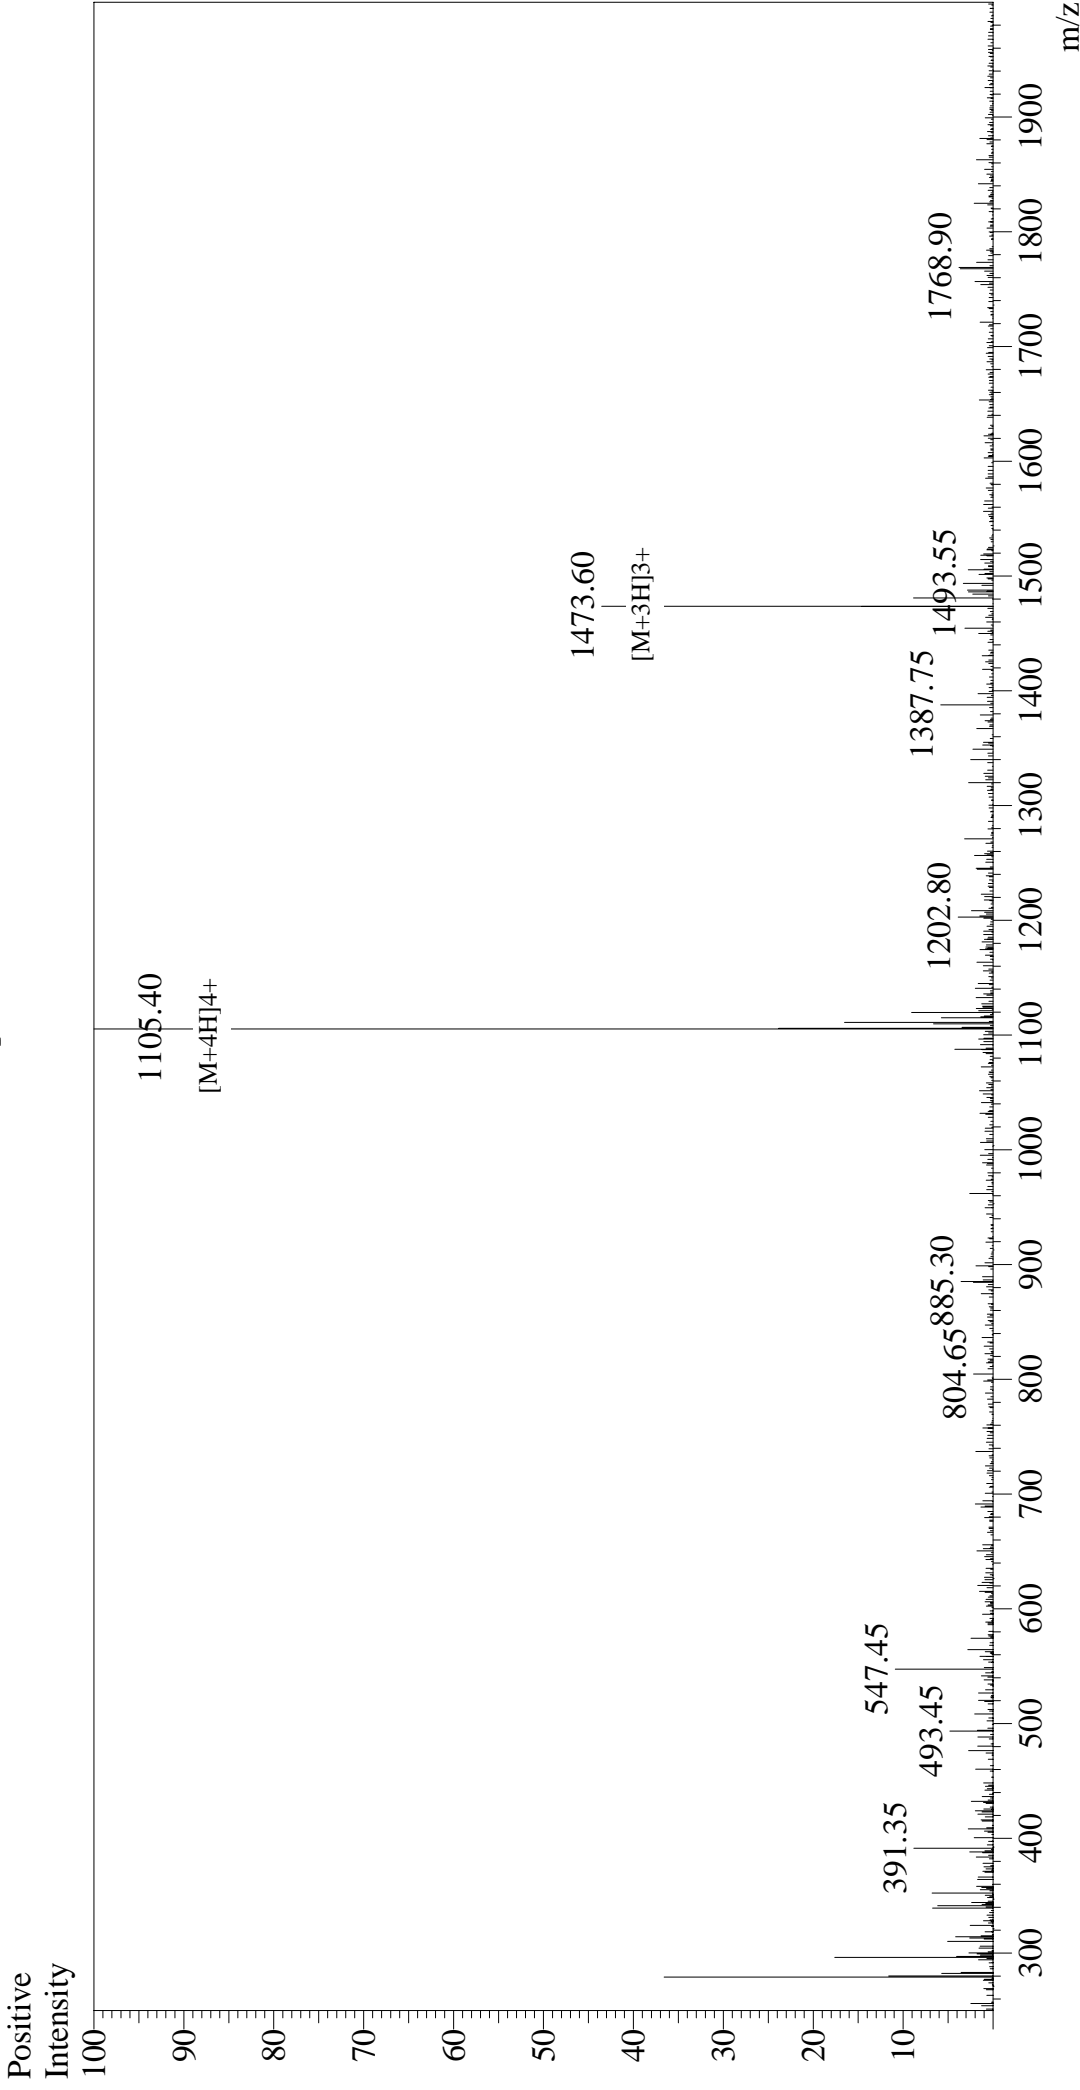

Sample Information

Acquired by : Gary
Month-Day Processed : 10/22/18
Time Processed : 12:29:25
Injection Volume : 0.4
Sample Name : β -Amyloid (1-42),rat
Cat No : RP10013
Lot No : PE8021810
Theoretical MW : 4418.10
Observed MW : 4417.60

Interface

Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH

Equipment : GK11010007