

Sample Name :Bim BH3, Peptide IV
 Cat No.: RP20339
 Lot No.: PE3891905
 Time Processed:16:15:48
 Month-Day-Year Processed:05/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

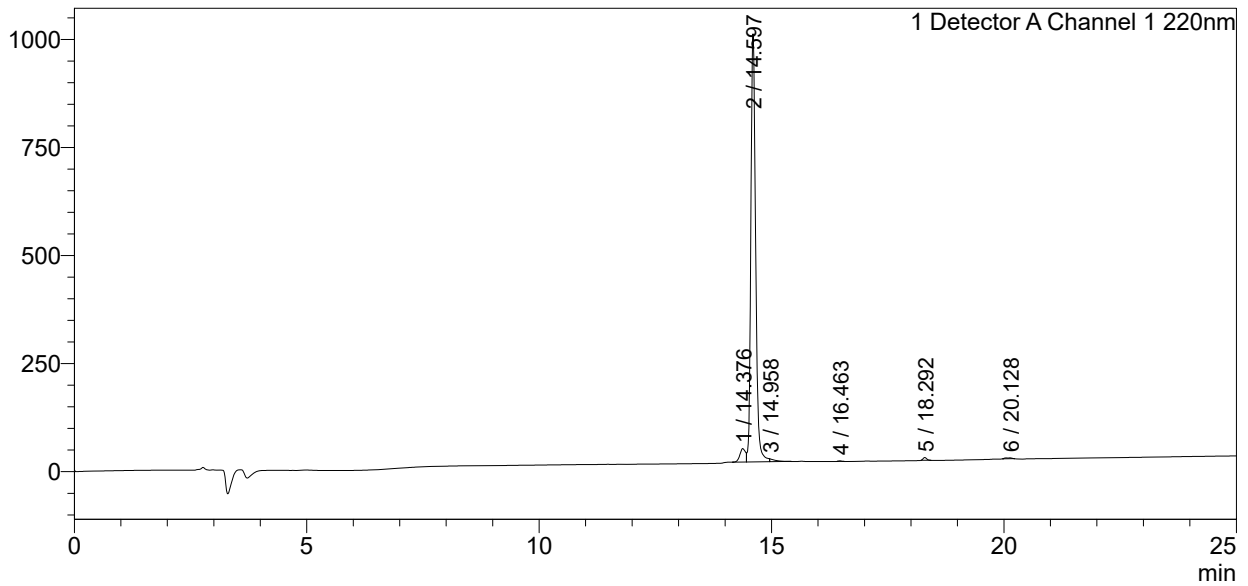

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.376	260388	30826	3.491
2	14.597	7086527	984917	95.002
3	14.958	53278	6839	0.714
4	16.463	5238	1171	0.070
5	18.292	32819	6019	0.440
6	20.128	21108	2030	0.283
Total		7459358	1031802	100.000