


# Mass Spectrum

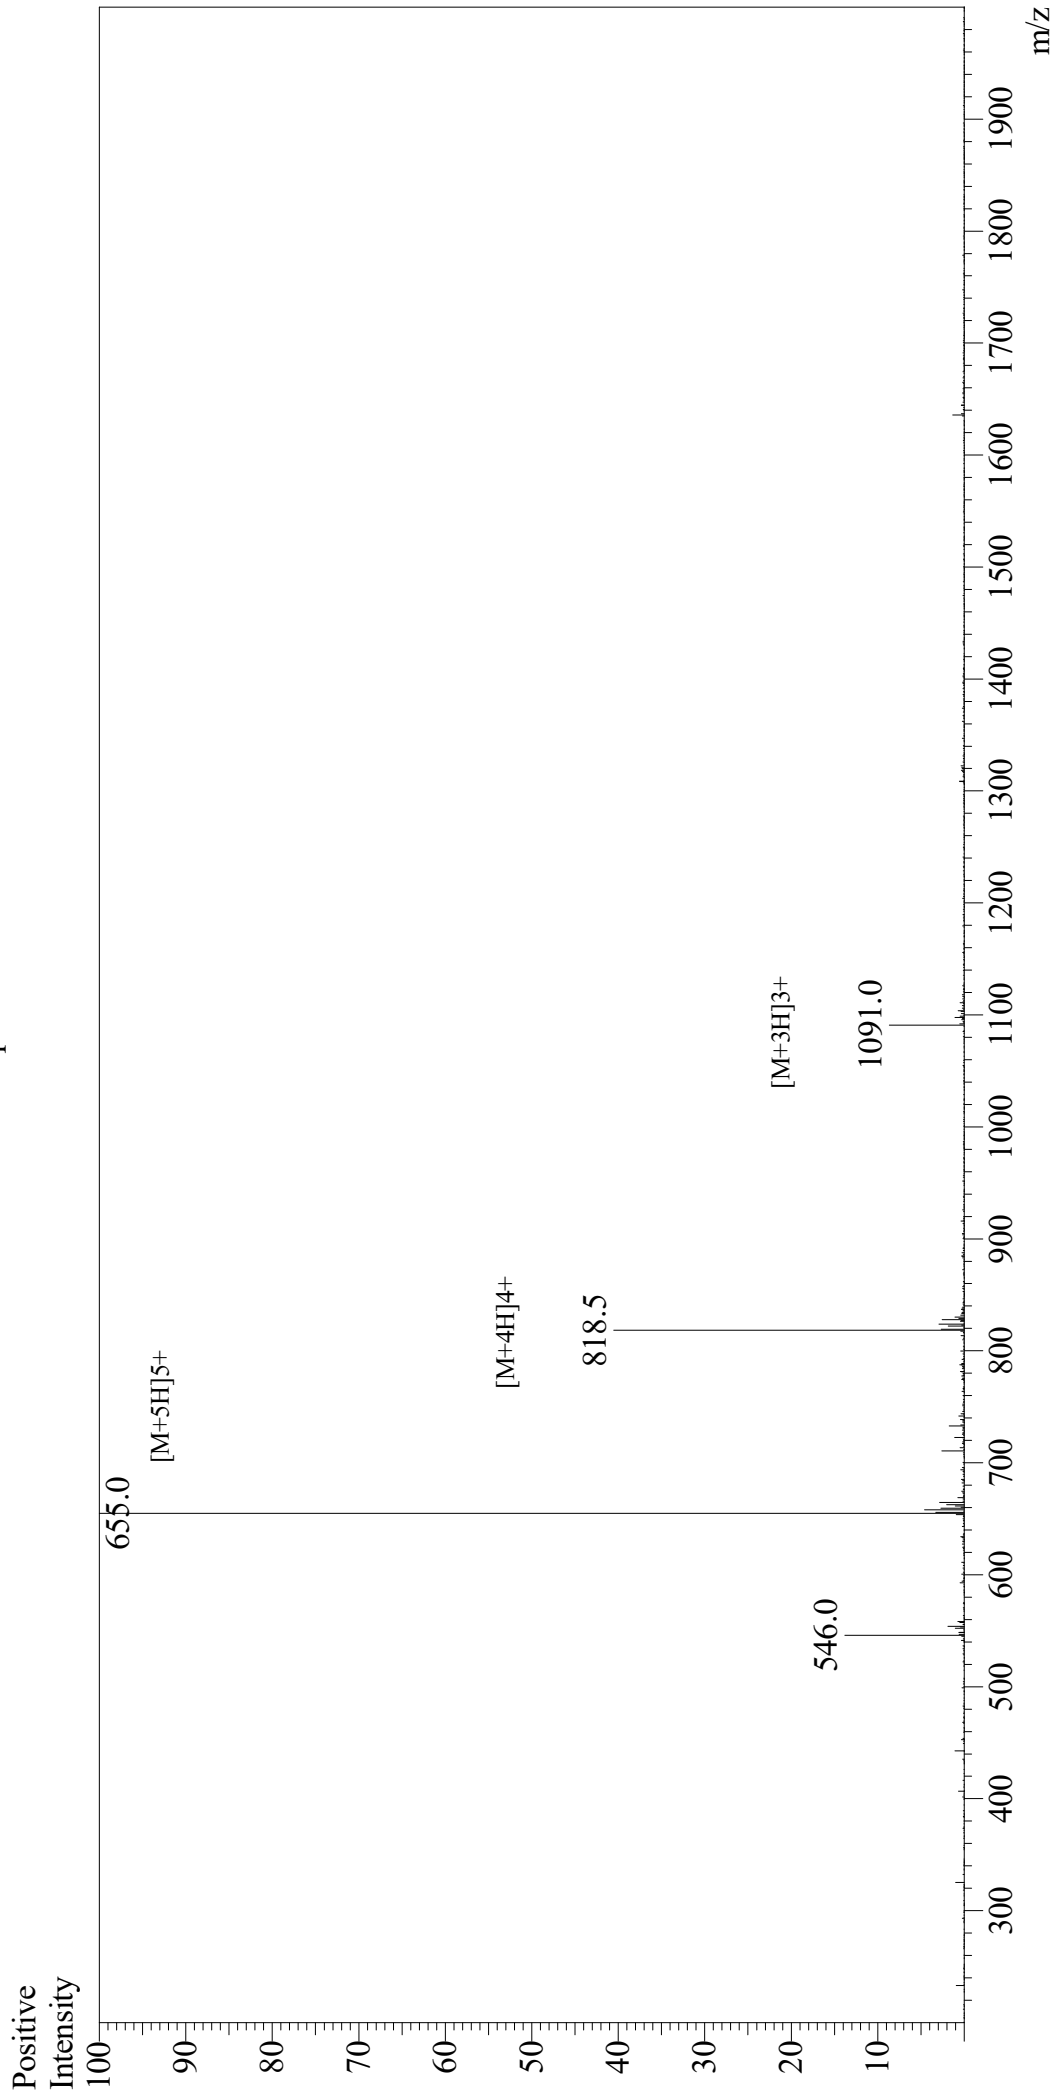

## Sample Information

User : Gary  
Month-Day Processed : 05/08/19  
Time Processed : 04:29:09 PM  
Injection Volume : 0.2  
Sample Name : Bim BH3, Peptide IV  
Cat No. : RP20339  
Lot No. : PE3891905  
Theoretical MW : 3269.70  
Observed MW : 3270.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH