

Sample Name :InsB 9-23

Cat. No. : RP20391

Lot. No. : PE3741804

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
95.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

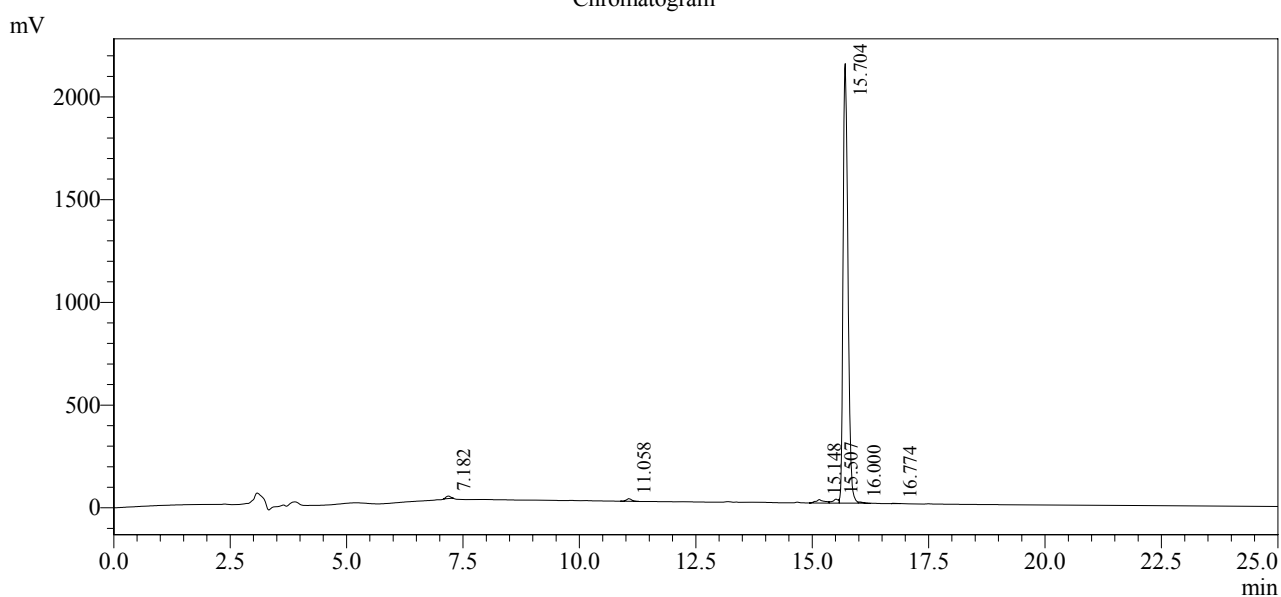

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.182	86279	12259	0.534
2	11.058	98240	12866	0.608
3	15.148	206782	16510	1.279
4	15.507	166853	18980	1.032
5	15.704	15552516	2138659	96.217
6	16.000	37371	5910	0.231
7	16.774	16030	2568	0.099
Total		16164072	2207752	100.000