

Sample Name :Amylin, human, amide
 Cat No. :RP11278
 Lot No. :E4900820K
 Time Processed : 7:55:46
 Month-Day-Year Processed : 11/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

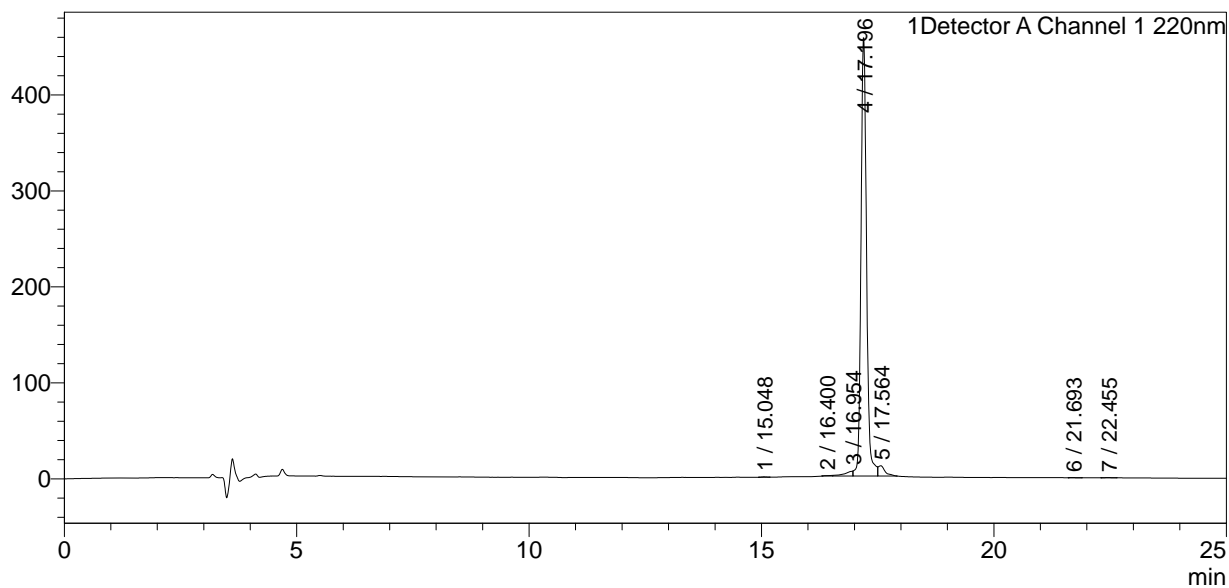

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.048	2245	323	0.057
2	16.400	6136	502	0.155
3	16.954	62054	4910	1.566
4	17.196	3783621	456339	95.455
5	17.564	106904	10694	2.697
6	21.693	509	81	0.013
7	22.455	2311	300	0.058
Total		3963780	473149	100.000