

Sample Name :Secretin, human
 Cat No: RP10249
 Lot No : E9466721H
 Time Processed :3:15:38
 Month-Day-Year Processed :08/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

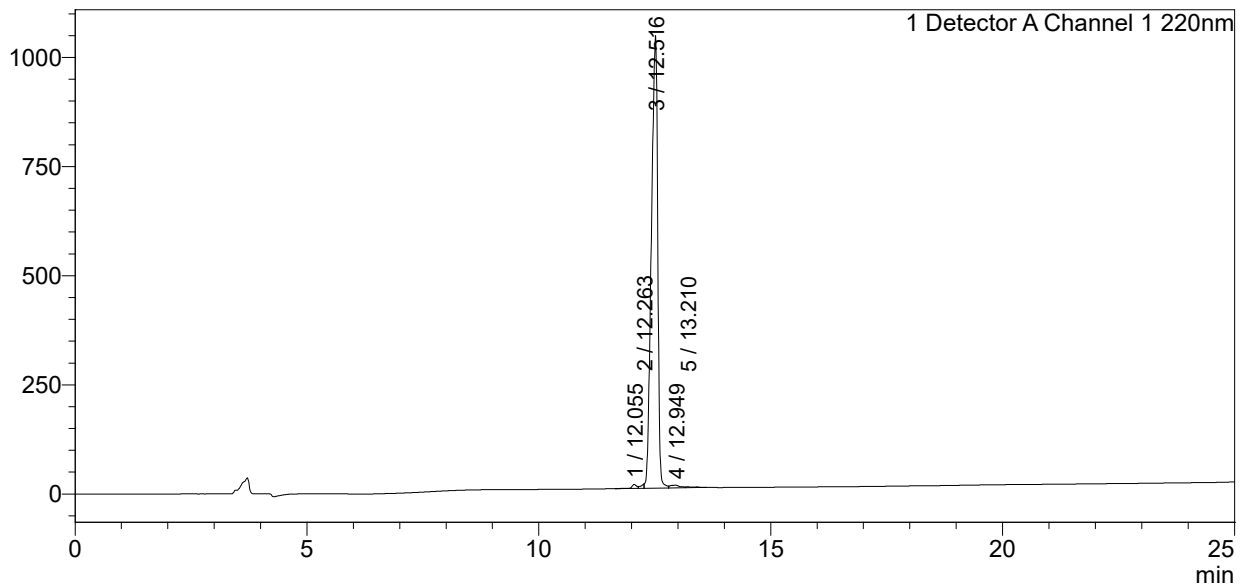

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 12.055 | 62572 | 9026 | 0.626 |
| 2 | 12.263 | 45499 | 9193 | 0.455 |
| 3 | 12.516 | 9783538 | 1036602 | 97.801 |
| 4 | 12.949 | 87372 | 6282 | 0.873 |
| 5 | 13.210 | 24492 | 1825 | 0.245 |
| Total | | 10003473 | 1062927 | 100.000 |