

Sample Name : Melittin
 Cat No. : RP10290
 Lot No. : PE5501612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
41.00	Pumps	Pump B Conc.	95
41.01	Pumps	Pump B Conc.	5
50.00	Pumps	Pump B Conc.	5
50.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

mV

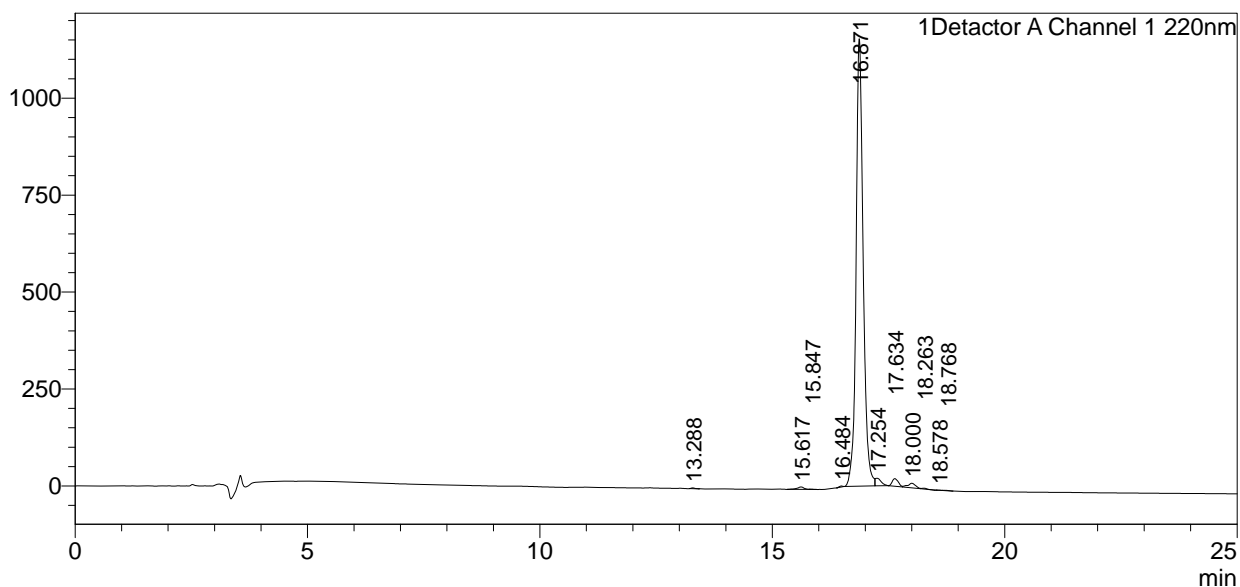

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.288	10482	1957	0.082
2	15.617	63944	6275	0.498
3	15.847	2934	536	0.023
4	16.484	14098	2463	0.110
5	16.871	12235774	1153385	95.277
6	17.254	167291	19534	1.303
7	17.634	179532	19623	1.398
8	18.000	139070	12073	1.083
9	18.263	17050	2396	0.133
10	18.578	3188	462	0.025
11	18.768	8925	1175	0.069
Total		12842287	1219877	100.000