

Sample Name :LL37 (Human)
 Cat. No. : RP13323
 Lot. No. : E7135021A

Time Processed :4:28:29
 Month-Day-Year Processed :01/15/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

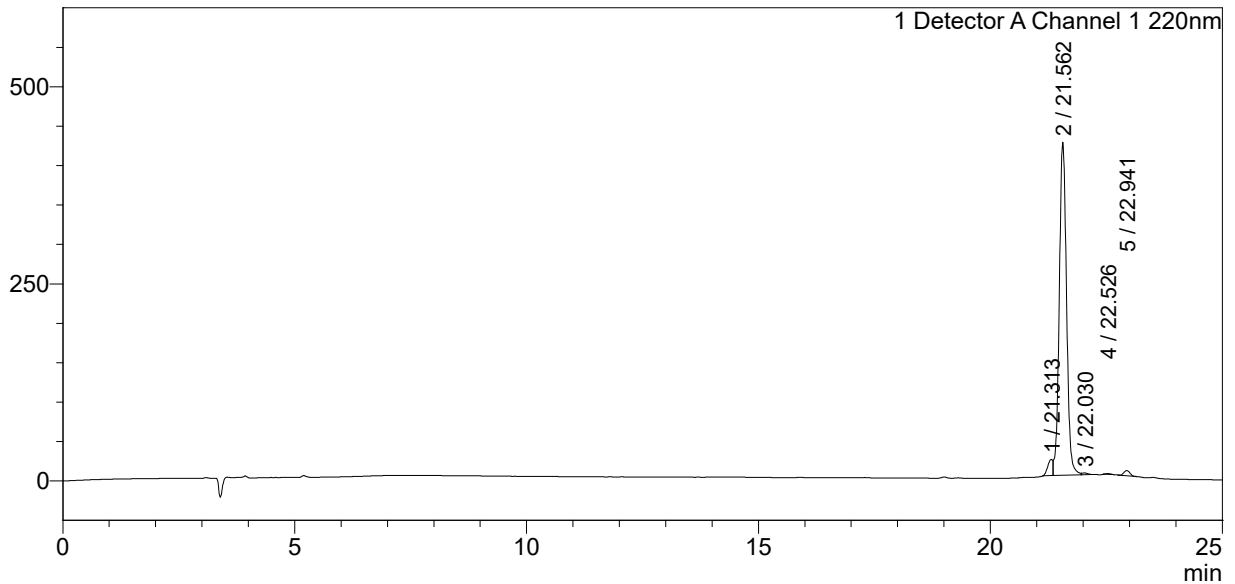

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.313	155691	20376	3.226
2	21.562	4586846	422286	95.042
3	22.030	17601	2112	0.365
4	22.526	7340	905	0.152
5	22.941	58665	6592	1.216
Total		4826144	452271	100.000