

Sample Name :Bradykinin (1-7)
 Cat No. :RP11133
 Lot No. :E2617320G
 Time Processed : 8:34:12
 Month-Day-Year Processed : 08/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

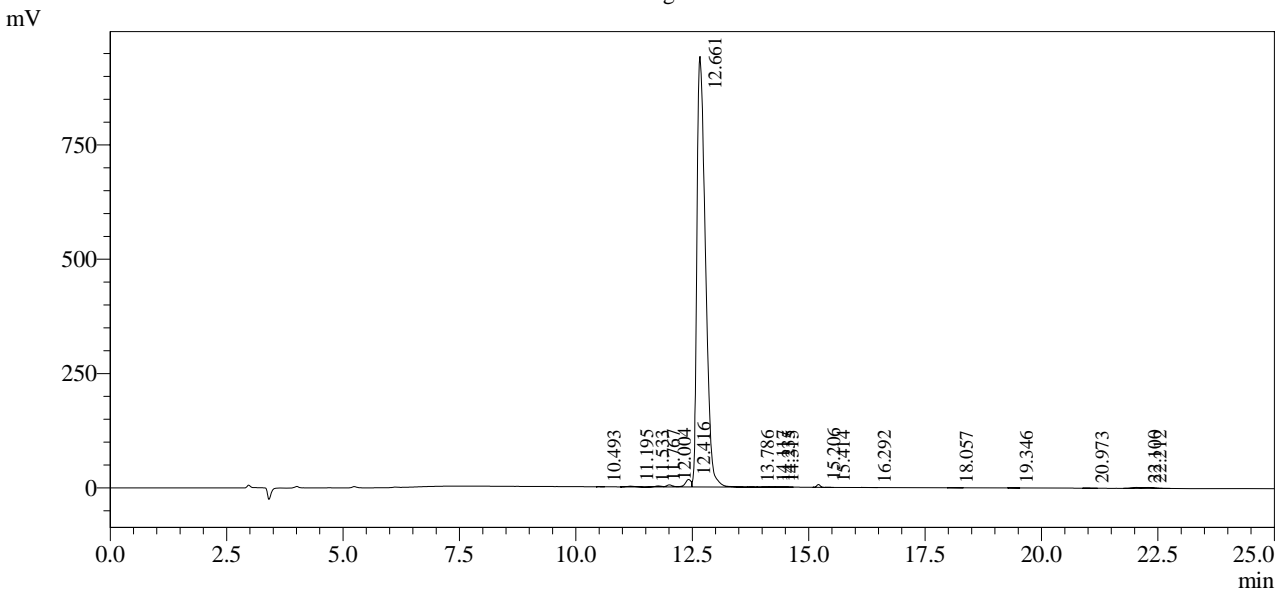

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.493	1251	229	0.010
2	11.195	18487	1651	0.150
3	11.533	2271	308	0.018
4	11.767	23092	2252	0.187
5	12.004	41119	4472	0.333
6	12.416	143932	16572	1.165
7	12.661	11996739	941702	97.139
8	13.786	2134	298	0.017
9	14.117	2759	296	0.022
10	14.235	2726	361	0.022
11	14.315	5001	367	0.040
12	15.206	32573	6088	0.264
13	15.414	1834	339	0.015
14	16.292	2677	276	0.022
15	18.057	1185	90	0.010
16	19.346	1112	155	0.009
17	20.973	2822	337	0.023
18	22.100	26652	2023	0.216
19	22.212	41712	2061	0.338
Total		12350080	979878	100.000