

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), human, porcine
 Cat No. :RP11927
 Lot No. :E8067221E
 Time Processed : 6:12:58 PM
 Month-Day-Year Processed : 06/11/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
65.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Atrial Natriuretic Peptide (ANP) (1-28), human, porcine

mV

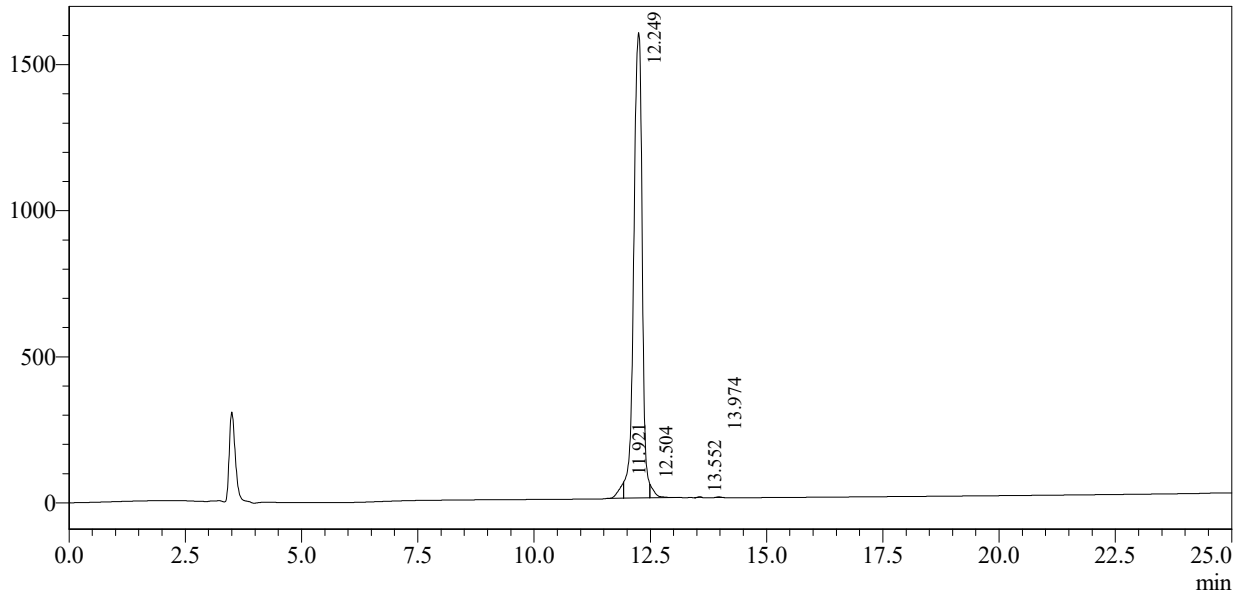

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.921	383872	52722	1.846
2	12.249	20101961	1593323	96.676
3	12.504	282854	43857	1.360
4	13.552	7719	1992	0.037
5	13.974	16658	2558	0.080
Total		20793064	1694452	100.000