

Sample Name : β -Amyloid (1-40)
 Cat No.: RP10004
 Lot No.: E7228820B
 Time Processed :19:08:16
 Month-Day-Year Processed :02/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

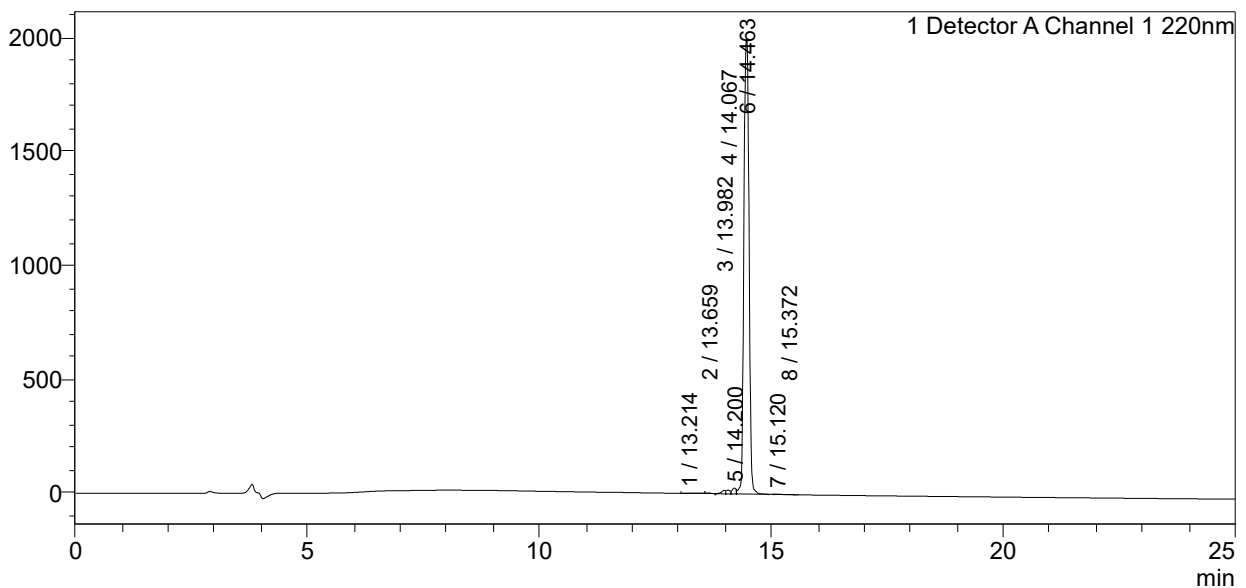

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.214	8298	426	0.053
2	13.659	12547	2197	0.079
3	13.982	101056	15362	0.640
4	14.067	84427	15918	0.535
5	14.200	168113	25760	1.065
6	14.463	15394032	2002680	97.539
7	15.120	9336	1210	0.059
8	15.372	4603	562	0.029
Total		15782412	2064114	100.000