

Sample Name :InsB 9-23
 Cat No. :RP20391
 Lot No. :E1587719I
 Time Processed :12:29:23
 Month-Day-Year Processed :09/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

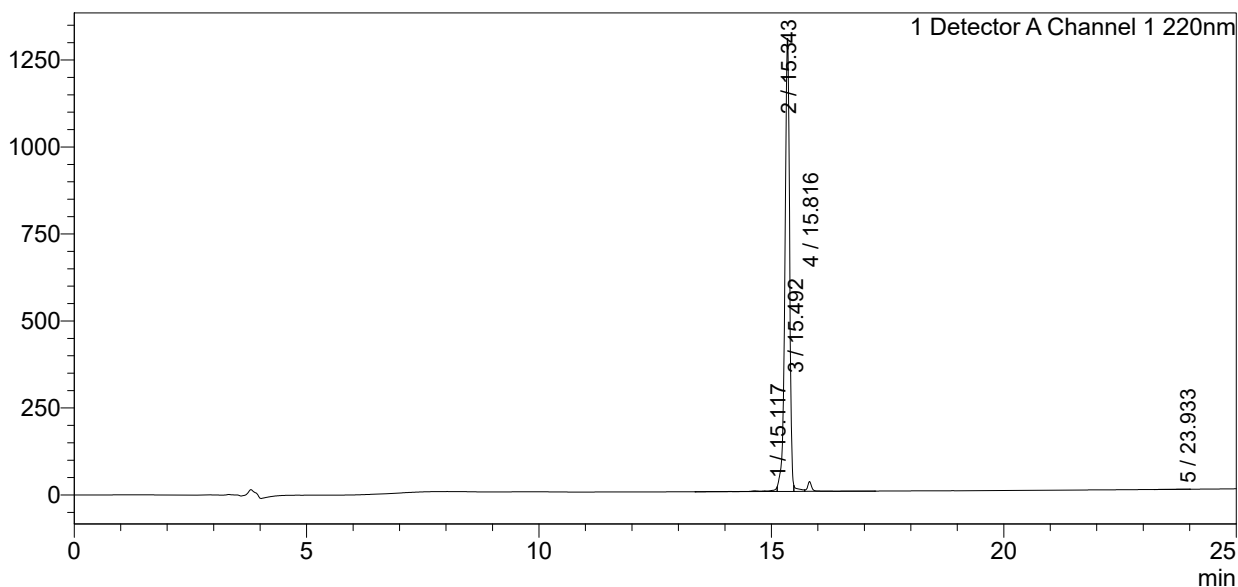

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.117	103464	10648	1.092
2	15.343	9098064	1301485	96.010
3	15.492	95561	13883	1.008
4	15.816	175311	28231	1.850
5	23.933	3793	65	0.040
Total		9476193	1354313	100.000