

Sample Name :DYKDDDDK Peptide  
 Cat No.: RP10586  
 Lot No.: E9676619J  
 Time Processed:8:25:05  
 Month-Day-Year Processed:10/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

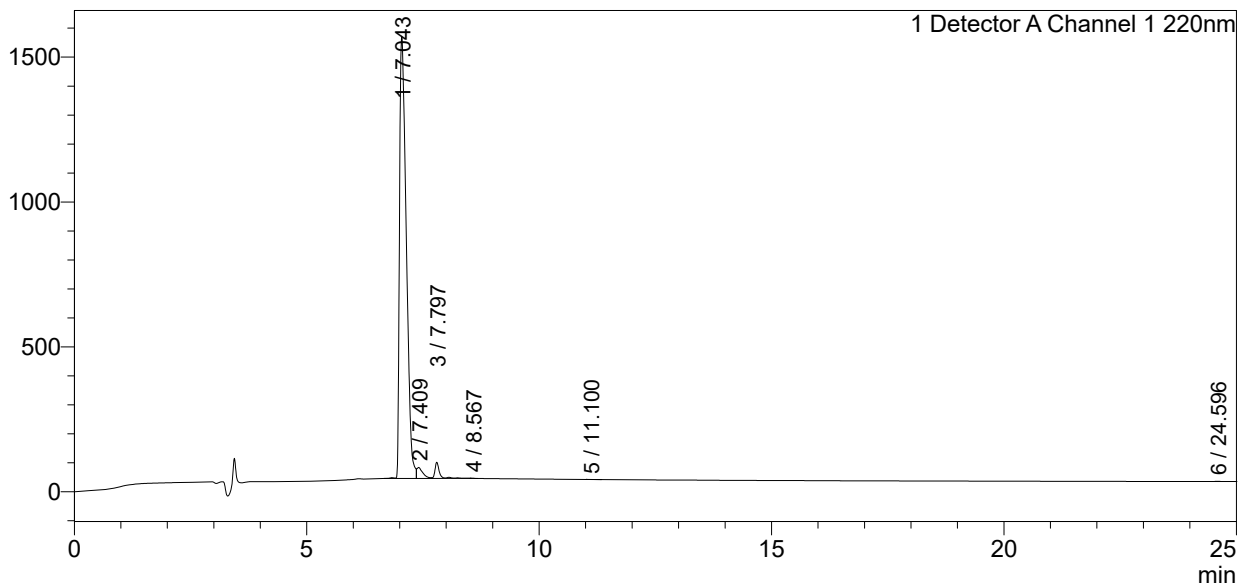

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.043	15384782	1526300	95.558
2	7.409	334704	37753	2.079
3	7.797	368617	55713	2.290
4	8.567	1093	284	0.007
5	11.100	3194	414	0.020
6	24.596	7595	851	0.047
Total		16099984	1621314	100.000