


Sample Name :Arg-Gly-Asp-Cys
 Cat. No. : RP10860
 Lot. No. : E5457819G
 Time Processed :14:12:11
 Month-Day-Year Processed : 07/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

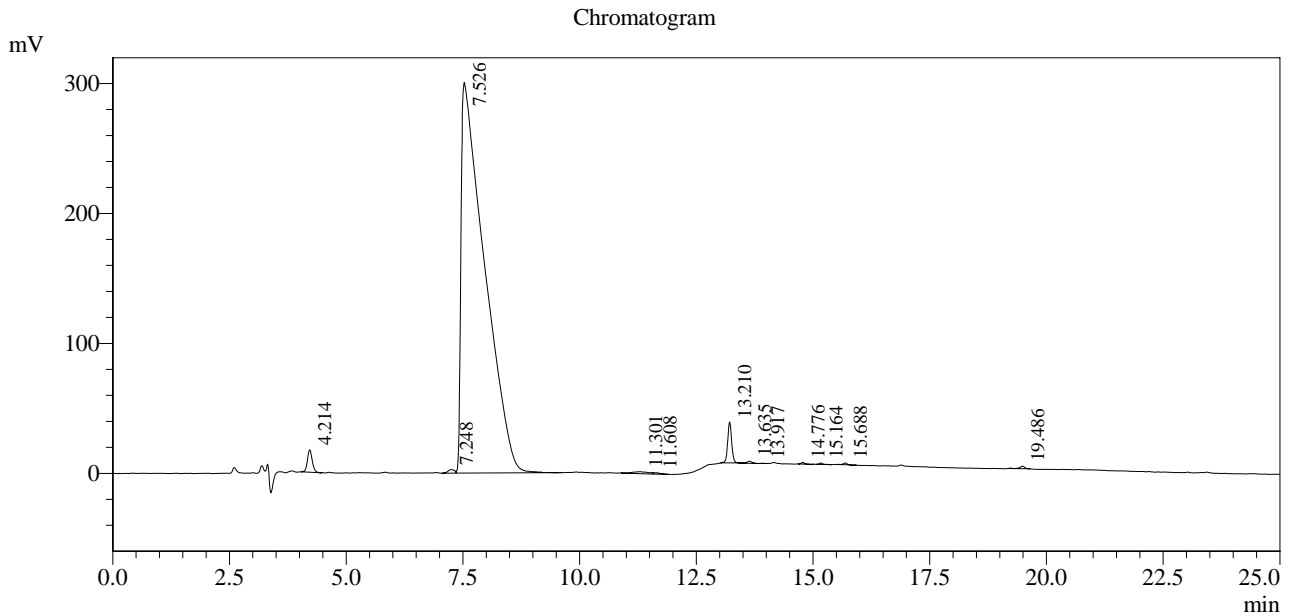

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.214	123096	17209	1.132
2	7.248	28352	2770	0.261
3	7.526	10444681	300580	96.026
4	11.301	37174	1562	0.342
5	11.608	11569	1045	0.106
6	13.210	185339	31437	1.704
7	13.635	12271	1544	0.113
8	13.917	948	203	0.009
9	14.776	5646	1275	0.052
10	15.164	6398	1119	0.059
11	15.688	6894	1395	0.063
12	19.486	14583	1964	0.134
Total		10876952	362102	100.000