

Sample Name :Melittin
 Cat No. :RP10290
 Lot No. :E7152220L
 Time Processed :11:53:04 PM
 Month-Day-Year Processed :12/26/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

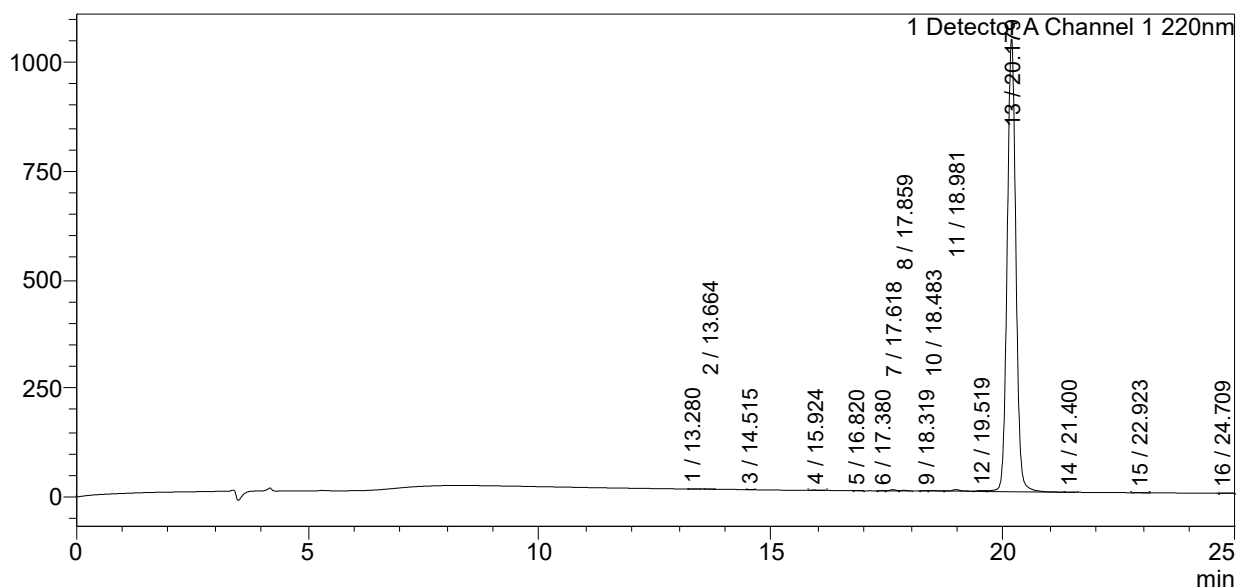

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.280	1720	267	0.013
2	13.664	3571	619	0.026
3	14.515	1089	211	0.008
4	15.924	7014	752	0.051
5	16.820	1623	195	0.012
6	17.380	3250	436	0.024
7	17.618	26000	2889	0.190
8	17.859	10377	1319	0.076
9	18.319	5398	641	0.039
10	18.483	9111	969	0.066
11	18.981	45328	3672	0.331
12	19.519	25560	2081	0.187
13	20.179	13558172	1042313	98.928
14	21.400	1717	274	0.013
15	22.923	3910	363	0.029

Peak#	Ret. Time	Area	Height	Area%
16	24.709	1248	137	0.009
Total		13705089	1057138	100.000