


Mass Spectrum

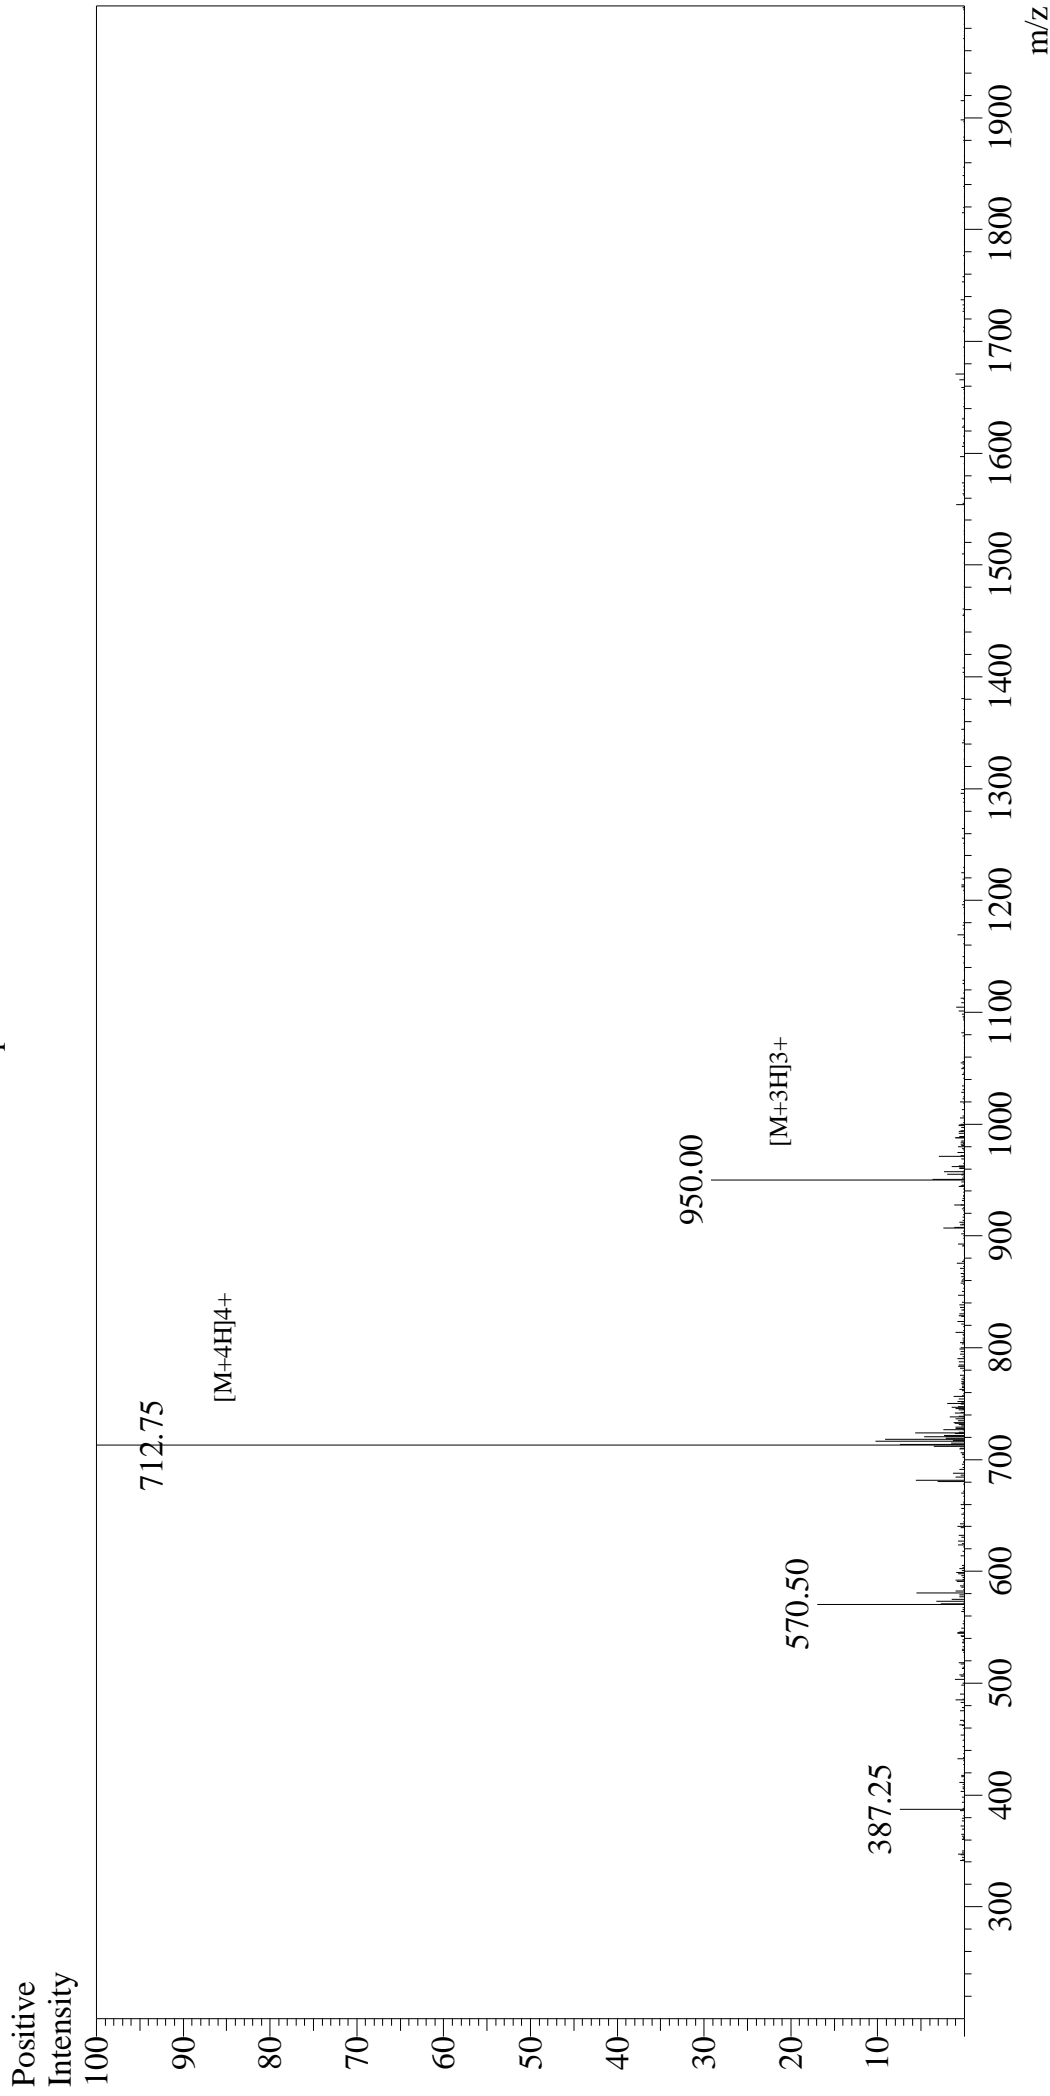

Sample Information

User : Gary
Month-Day Processed : 03/05/18
Time Processed : 14:48:52
Injection Volume : 0.2
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : PE4101802
Theoretical MW : 2847.5
Observed MW : 2847.00

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH