

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : E2666321E

Time Processed: 11:01:48
 Year-Month-Day: 2021/5/9

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	0	
5.00	Pumps	Solvent B Conc.	0	
20.00	Pumps	Solvent B Conc.	30	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
30.00	Pumps	Solvent B Conc.	95	
30.01	Pumps	Solvent B Conc.	0	
40.00	Pumps	Solvent B Conc.	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

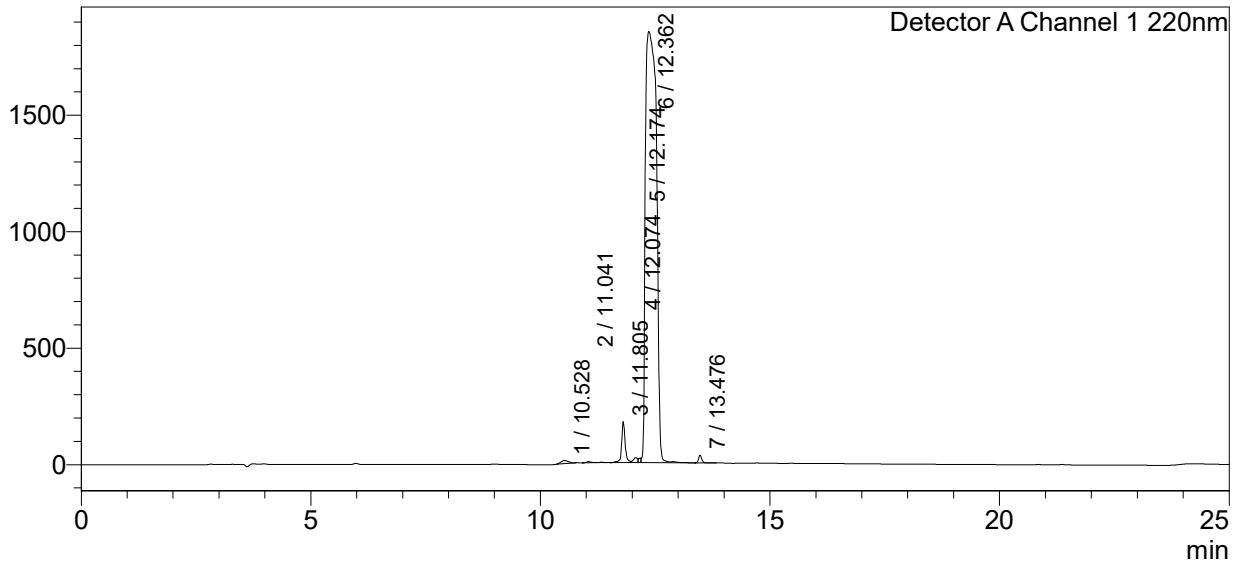

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.528	142366	12783	0.443
2	11.041	30893	5094	0.096
3	11.805	959582	176438	2.983
4	12.074	139070	21837	0.432
5	12.174	74586	19635	0.232
6	12.362	30672845	1851889	95.339
7	13.476	152912	32881	0.475
Total		32172254	2120558	100.000