

Sample Name: DYKDDDDK Peptide  
 Cat No. : RP10586  
 Lot No. : E3993621F  
 Time Processed : 7:17:46 AM  
 Month-Day-Year Processed : 06/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
5.00	Pumps	Pump A B.Conc	0
20.00	Pumps	Pump A B.Conc	30
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	0
35.00	Pumps	Pump A B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

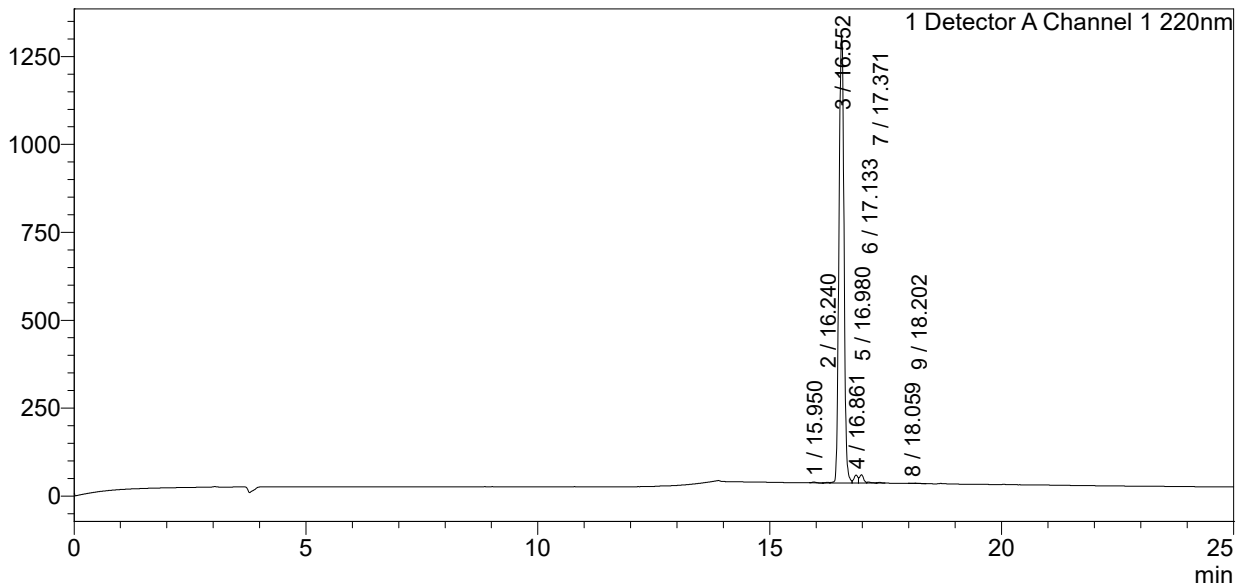

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.950	13548	2390	0.137
2	16.240	10085	1658	0.102
3	16.552	9512339	1275099	96.537
4	16.861	138021	23052	1.401
5	16.980	143737	23824	1.459
6	17.133	17877	2759	0.181
7	17.371	10941	2101	0.111
8	18.059	2259	570	0.023
9	18.202	4768	968	0.048
Total		9853574	1332422	100.000