

Sample Name : InsB 9-23
 Cat. No. : RP20391
 Lot. No. : PE2741611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

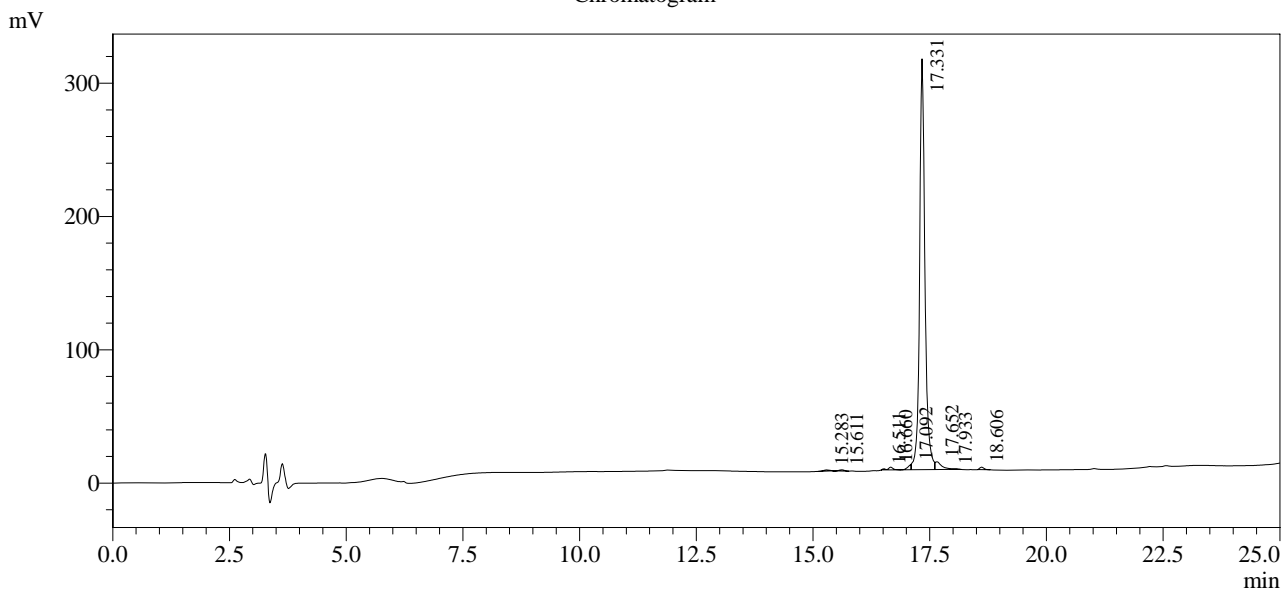

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.283	9077	898	0.350
2	15.611	7090	959	0.273
3	16.511	4220	886	0.163
4	16.660	12469	2046	0.481
5	17.092	19263	3956	0.743
6	17.331	2469290	308187	95.233
7	17.652	54963	5754	2.120
8	17.933	5380	566	0.207
9	18.606	11147	1792	0.430
Total		2592899	325044	100.000