

Sample Name : PAR-4 Agonist Peptide, amide
 Cat. No. : RP11529
 Lot. No. : PE8431902
 Time Processed : 10:07:08
 Month-Day-Year Processed : 03/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

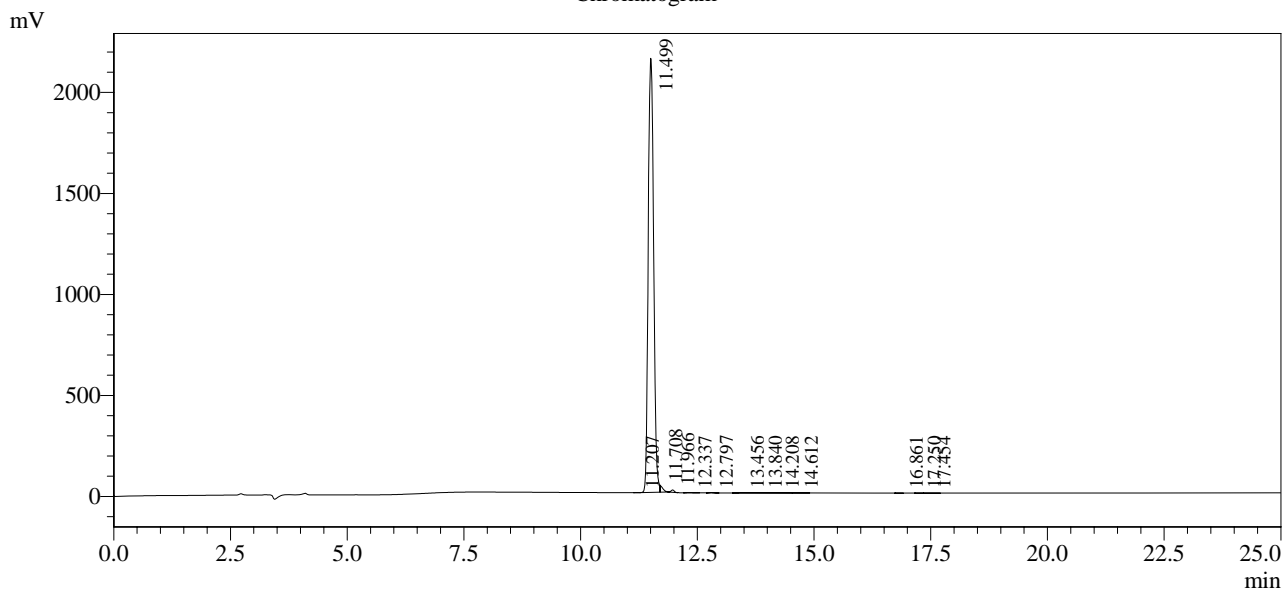

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.207	576	142	0.003
2	11.499	17359687	2149251	98.383
3	11.708	133873	32650	0.759
4	11.966	54477	11748	0.309
5	12.337	6422	846	0.036
6	12.797	11078	1956	0.063
7	13.456	5725	580	0.032
8	13.840	15657	850	0.089
9	14.208	39178	1780	0.222
10	14.612	9224	610	0.052
11	16.861	1012	114	0.006
12	17.250	1340	146	0.008
13	17.454	6727	776	0.038
Total		17644975	2201449	100.000