

Sample Name :Bradykinin  
Cat No. :RP11129  
Lot No. :E3688720E  
Time Processed :9:12:29  
Month-Day-Year Processed :05/24/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
Equipment: ZJ17010508

### <Chromatogram>

mV

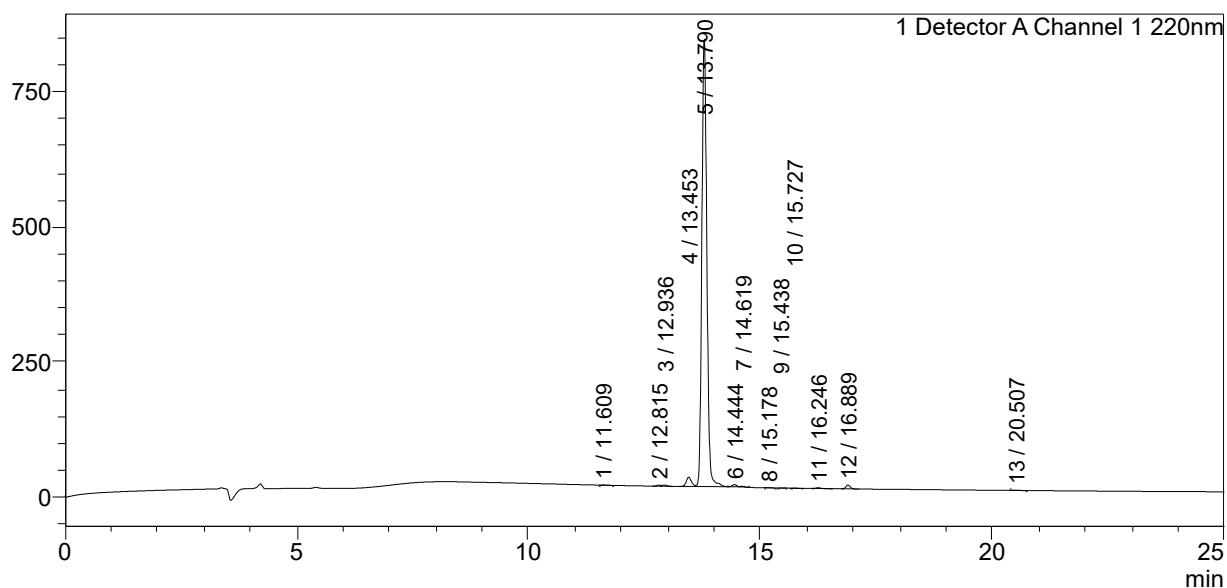

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.609	2647	385	0.041
2	12.815	13111	2114	0.203
3	12.936	14698	2244	0.228
4	13.453	134443	17320	2.084
5	13.790	6192425	827962	95.982
6	14.444	24692	3821	0.383
7	14.619	5085	989	0.079
8	15.178	2053	264	0.032
9	15.438	1224	239	0.019
10	15.727	1771	212	0.027
11	16.246	11277	1654	0.175
12	16.889	46510	7096	0.721
13	20.507	1746	161	0.027
Total		6451682	864462	100.000